


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010716\
 Data File : BF084303.D
 Acq On : 7 Jan 2016 9:35
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

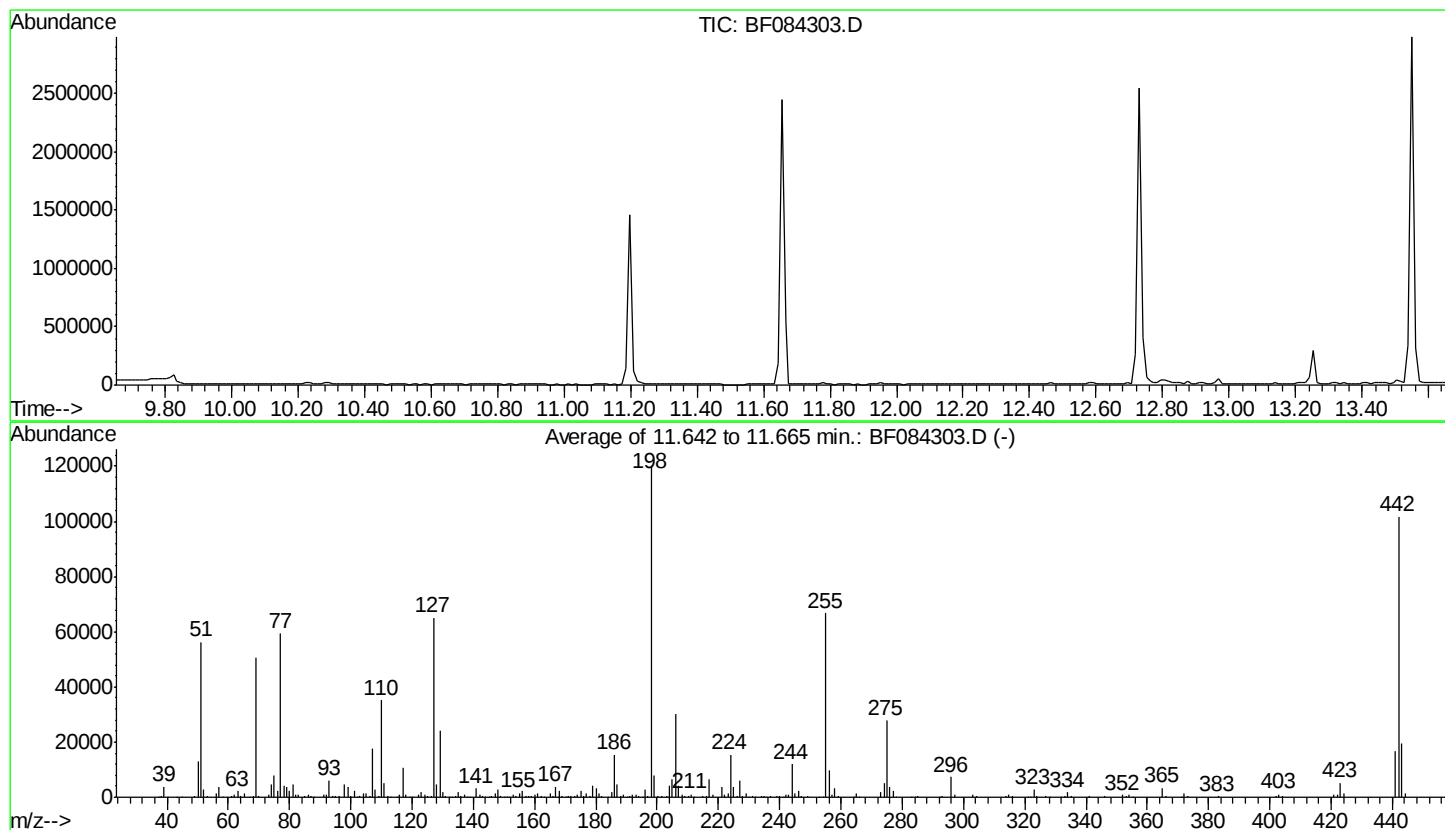

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	56229	PASS
68	69	0.00	2	1.2	599	PASS
69	198	0.00	100	42.2	50723	PASS
70	69	0.00	2	0.8	412	PASS
127	198	10	80	54.2	65102	PASS
197	198	0.00	2	0.4	527	PASS
198	198	100	100	100.0	120224	PASS
199	198	5	9	6.7	8111	PASS
275	198	10	60	23.1	27745	PASS
365	198	1	100	2.9	3482	PASS
441	442	0.01	24	16.5	16786	PASS
442	198	50	100	84.6	101726	PASS
443	442	15	24	19.2	19512	PASS