
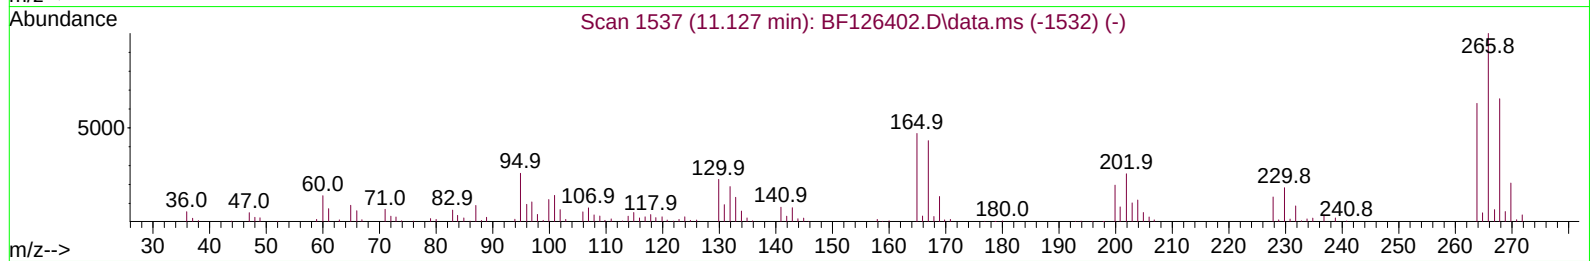
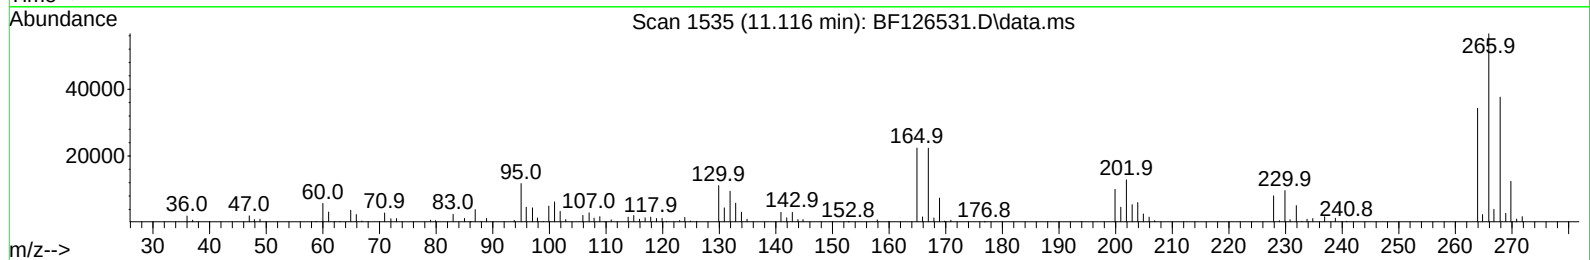


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
Data File : BF126531.D
Acq On : 7 Jan 2022 10:21
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 15:18:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 01:57:07 2022
Response via : Initial Calibration

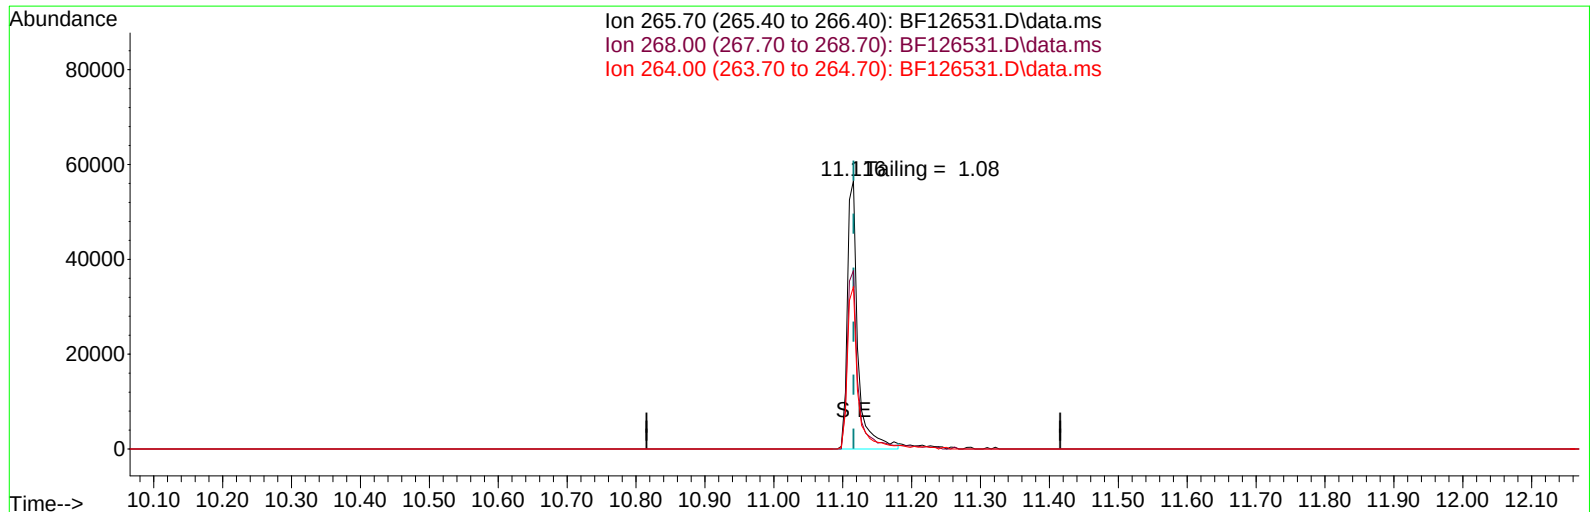

TIC: BF126531.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.000) 52964.56 ng

response 59800

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.50
264.00	63.00	60.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
Data File : BF126531.D
Acq On : 7 Jan 2022 10:21
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 07 15:18:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 01:57:07 2022
Response via : Initial Calibration

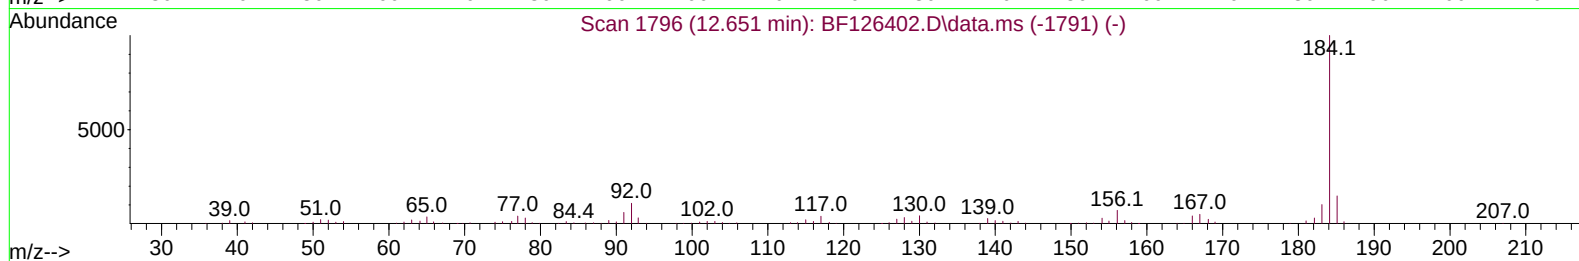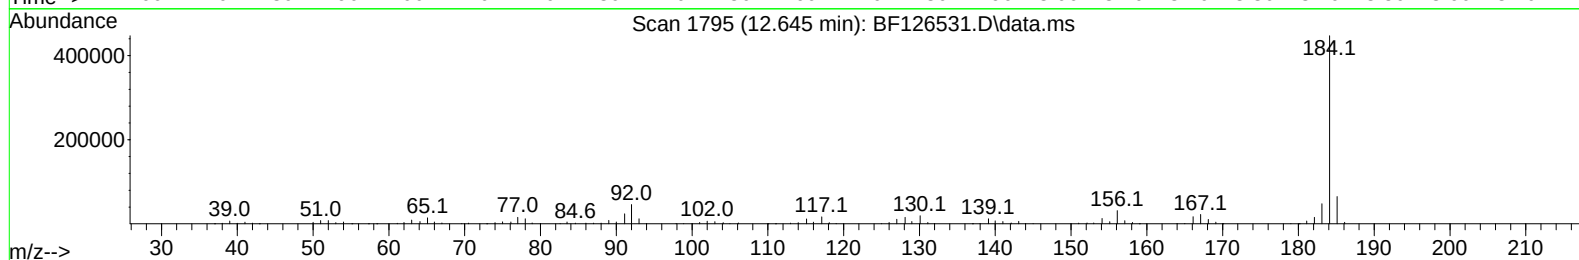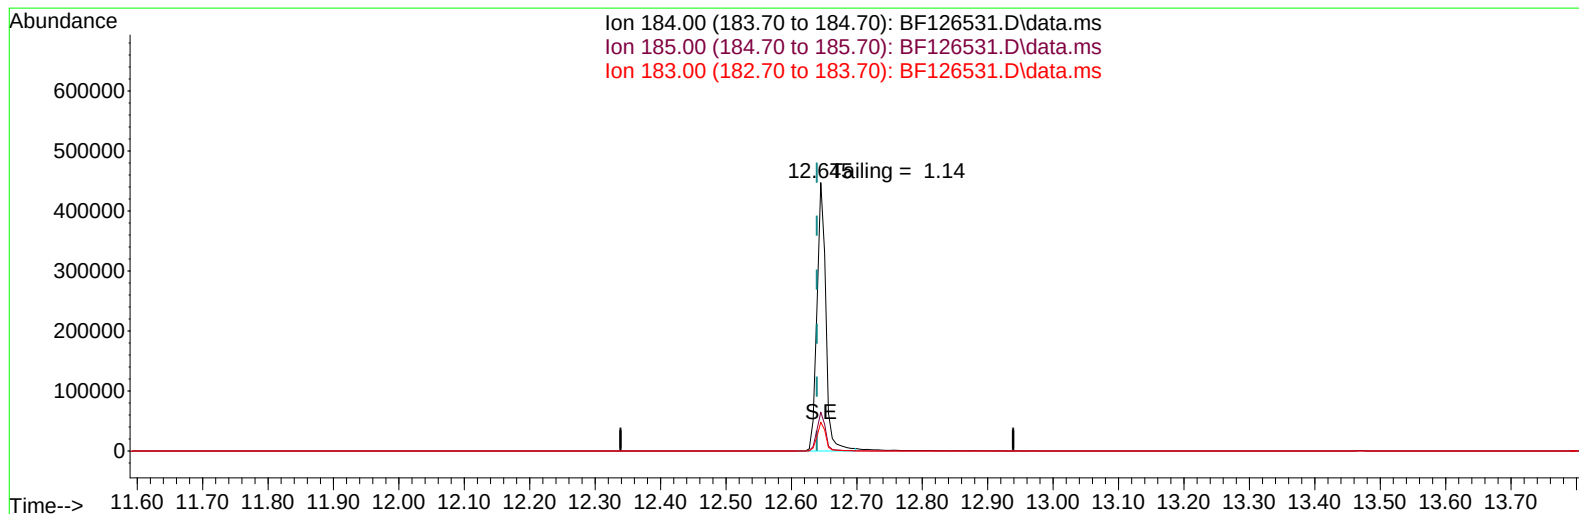

TIC: BF126531.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 0.00 ng

response 431538

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.52
183.00	10.20	10.73
0.00	0.00	0.00