

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
 Data File : BF126538.D
 Acq On : 7 Jan 2022 13:29
 Operator : JU/CG
 Sample : PB141875BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB141875BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	494	498	506	rVB	24217	32486	1.15%	0.179%
2	5.404	558	564	567	rBV	2632868	2778224	98.11%	15.330%
3	6.416	730	736	739	rBV	2498893	2814070	99.37%	15.528%
4	6.775	794	797	801	rBV	636848	581716	20.54%	3.210%
5	7.345	888	894	897	rBV	1735261	1901124	67.13%	10.490%
6	8.063	1011	1016	1019	rBV	853142	808084	28.54%	4.459%
7	9.145	1194	1200	1203	rBV	2714050	2831833	100.00%	15.626%
8	9.816	1309	1314	1318	rBV	905228	813644	28.73%	4.490%
9	10.610	1444	1449	1452	rBV	1671304	1527076	53.93%	8.426%
10	11.304	1563	1567	1571	rBV	891311	740294	26.14%	4.085%
11	12.898	1833	1838	1841	rBV	2275703	2133427	75.34%	11.772%
12	13.945	2013	2016	2025	rBV	458732	454176	16.04%	2.506%
13	14.045	2027	2033	2043	rBV	27207	31176	1.10%	0.172%
14	15.068	2202	2207	2213	rBV	28699	29609	1.05%	0.163%
15	15.398	2258	2263	2267	rBV	346416	421104	14.87%	2.324%
16	15.439	2267	2270	2276	rVB	39779	48592	1.72%	0.268%
17	15.862	2336	2342	2349	rBV	30866	47398	1.67%	0.262%
18	16.357	2421	2426	2434	rBV	29116	50091	1.77%	0.276%
19	16.939	2517	2525	2530	rBV2	18875	37125	1.31%	0.205%
20	17.621	2631	2641	2648	rBV5	16162	41884	1.48%	0.231%




Sum of corrected areas: 18123133

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
Data File : BF126538.D
Acq On : 7 Jan 2022 13:29
Operator : JU/CG
Sample : PB141875BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

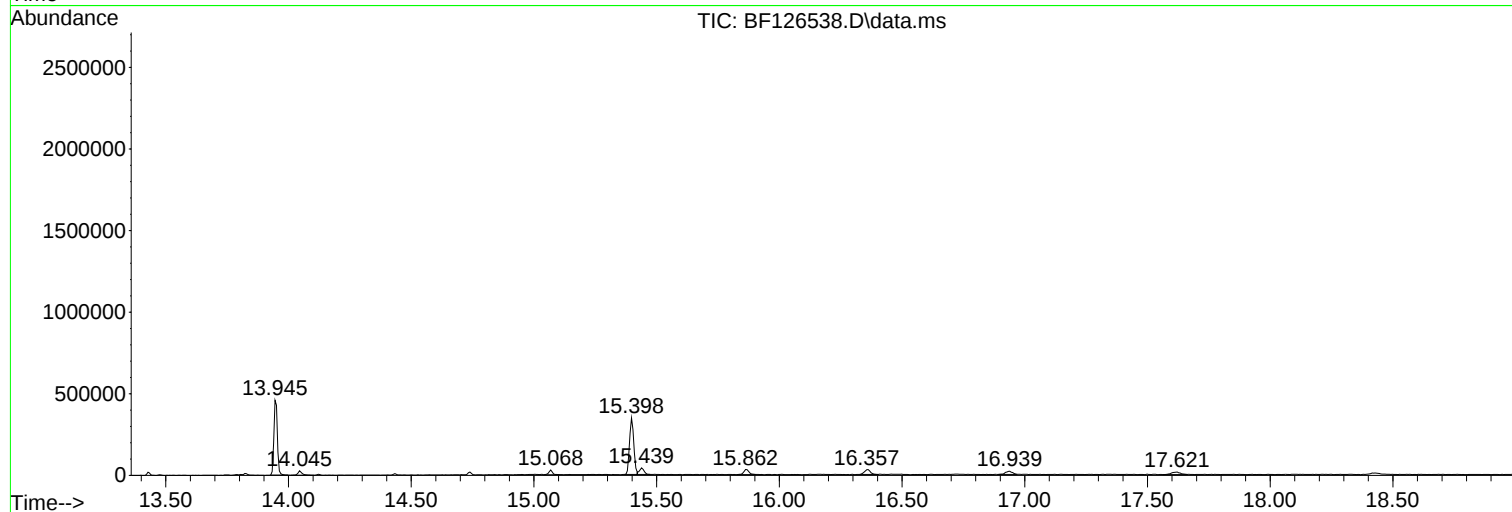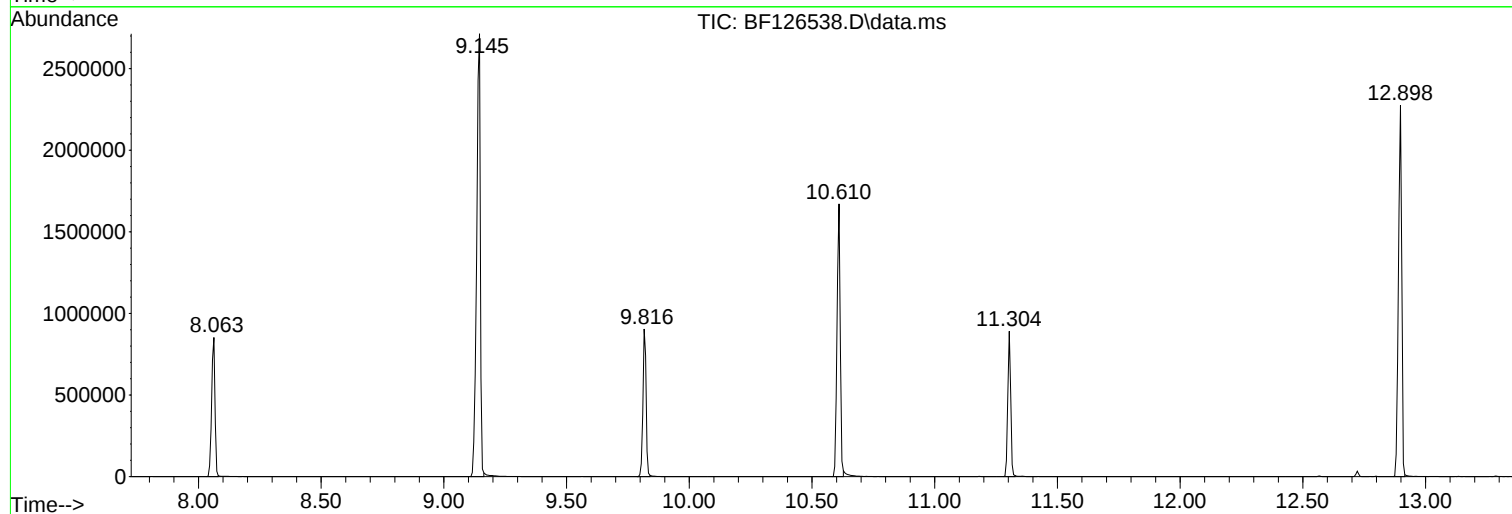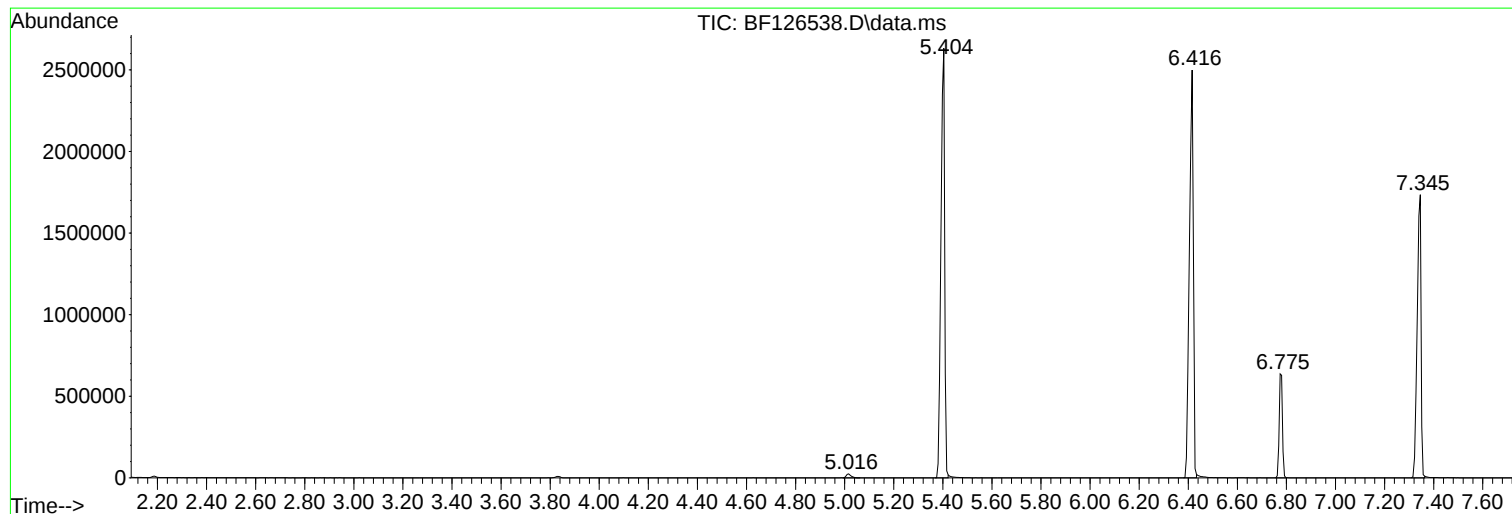

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
Data File : BF126538.D
Acq On : 7 Jan 2022 13:29
Operator : JU/CG
Sample : PB141875BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
Data File : BF126538.D
Acq On : 7 Jan 2022 13:29
Operator : JU/CG
Sample : PB141875BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141875BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------