
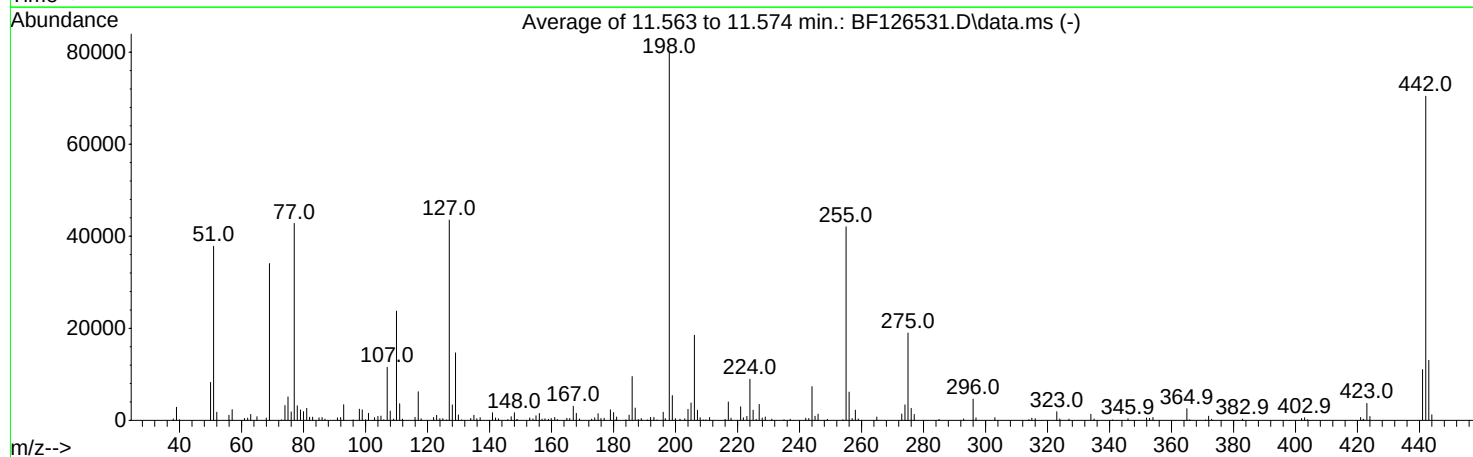


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
 Data File : BF126531.D
 Acq On : 7 Jan 2022 10:21
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 10 14:50:31 2022

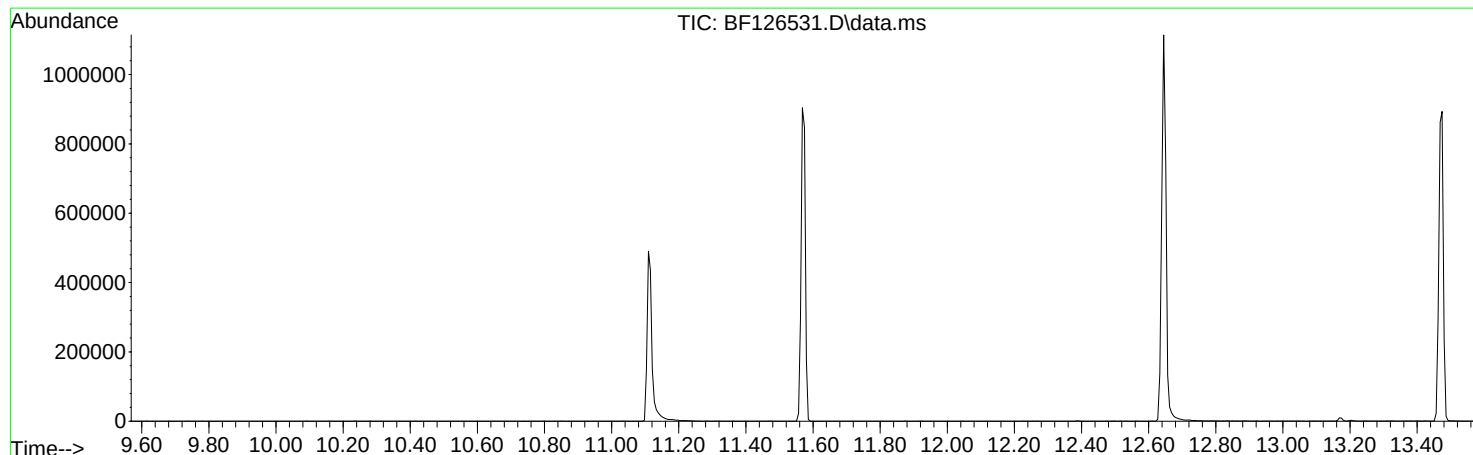




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.3	37811	PASS
68	69	0.00	2	1.6	538	PASS
69	198	0.00	100	42.6	34056	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.5	43525	PASS
197	198	0.00	2	0.5	392	PASS
198	198	100	100	100.0	79920	PASS
199	198	5	9	6.7	5391	PASS
275	198	10	60	23.8	18999	PASS
365	198	1	100	3.2	2555	PASS
441	198	0.01	100	13.8	11011	PASS
442	442	50	100	100.0	70444	PASS
443	442	15	24	18.5	13045	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
 Data File : BF126531.D
 Acq On : 7 Jan 2022 10:21
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 07 15:18:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 05 01:57:07 2022
 Response via : Initial Calibration

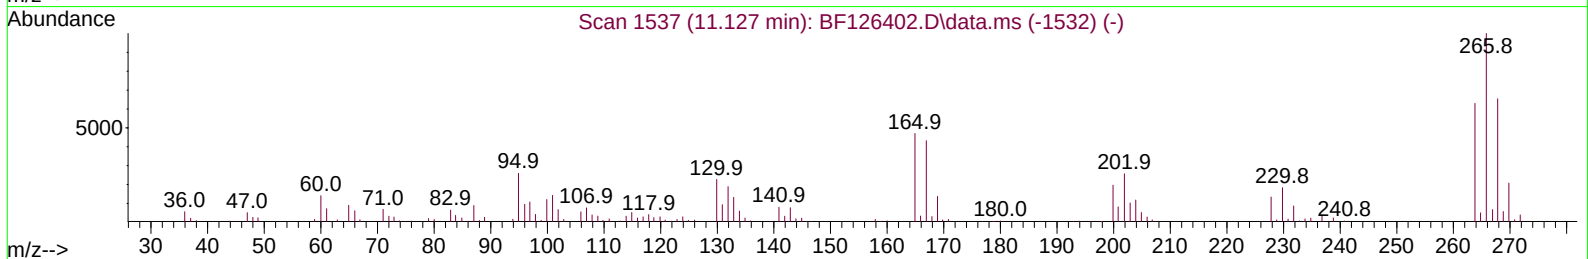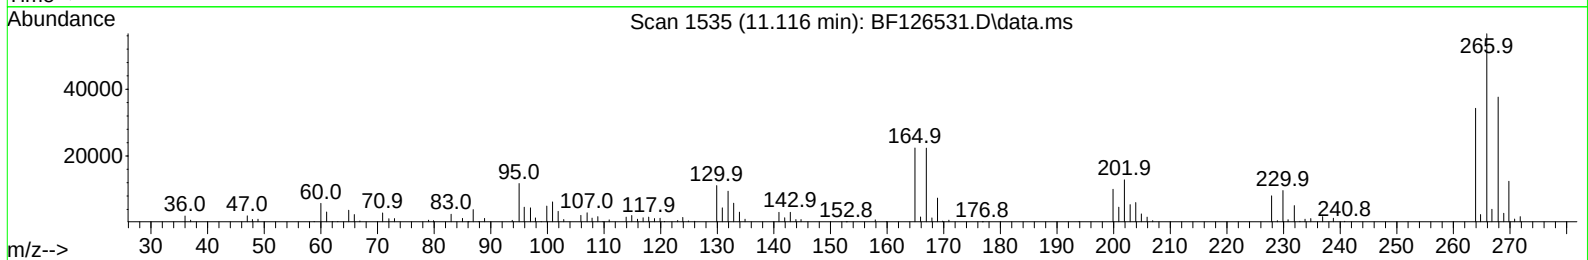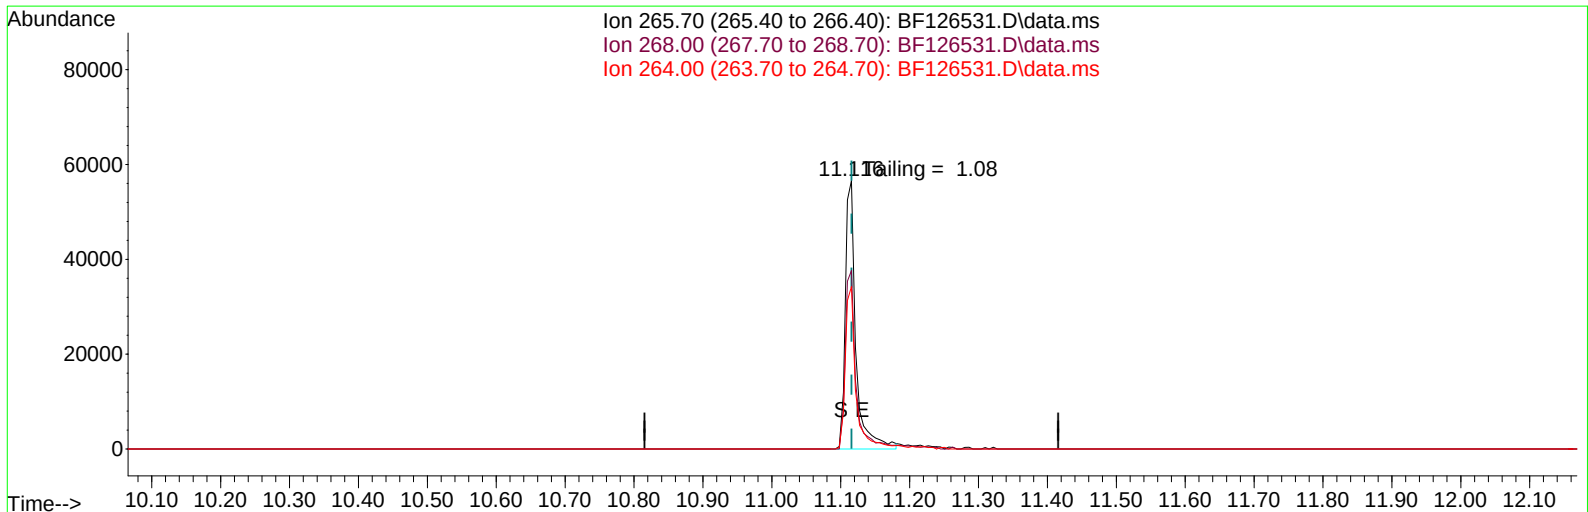

TIC: BF126531.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.000) 52964.56 ng




response 59800

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.50
264.00	63.00	60.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010722\
Data File : BF126531.D
Acq On : 7 Jan 2022 10:21
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 07 15:18:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 05 01:57:07 2022
Response via : Initial Calibration

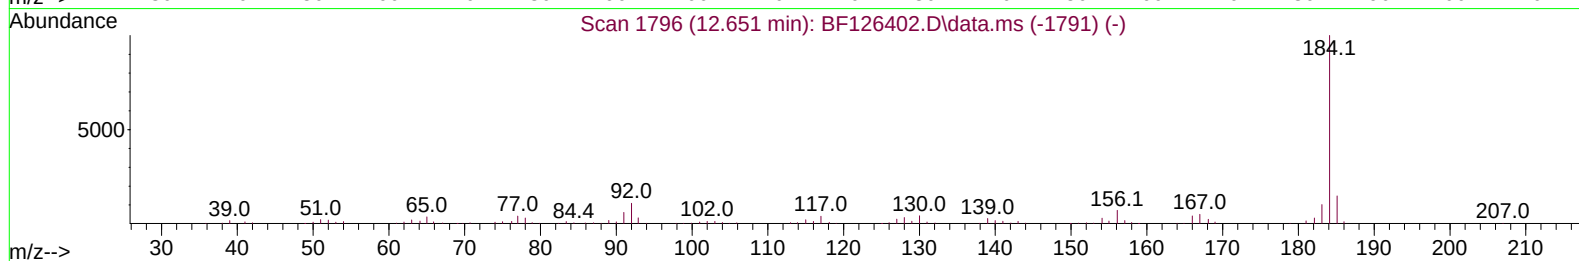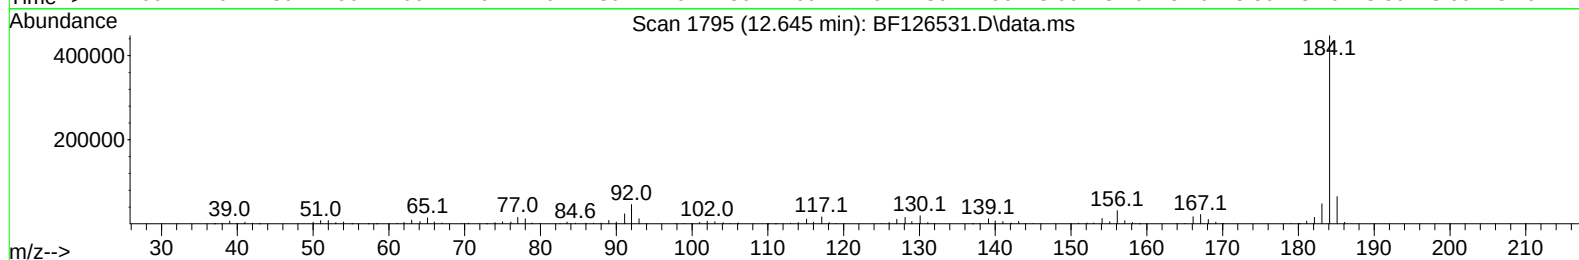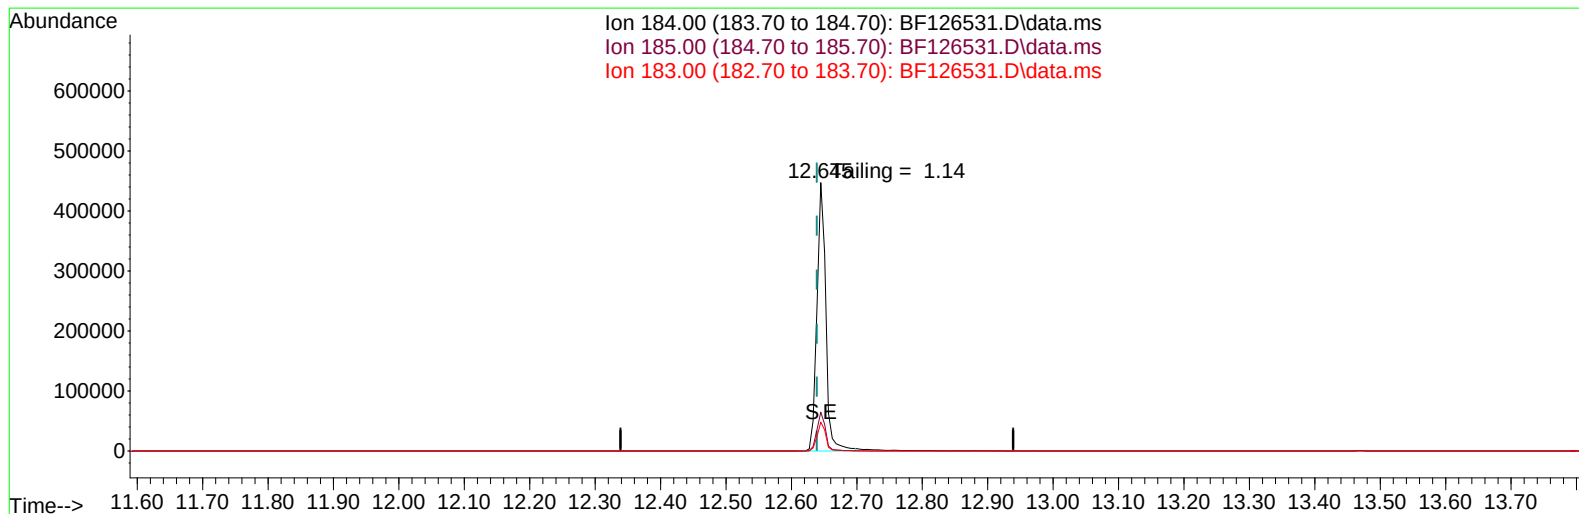

TIC: BF126531.D\data.ms

(77) Benzidine

12.645min (+ 0.006) 0.00 ng

response 431538

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.52
183.00	10.20	10.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/7/2022	BNA_F	<u>BF126531.D</u>
Compound Name	Response	Retention Time
DDT	162158	13.47
DDD	2950	13.17
DDE	258	12.83
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3208	165366	1.94