


Data Path : Z:\HPCHEM1\BNA F\Data\BF010816\
Data File : BF084326.D
Acq On : 8 Jan 2016 11:09
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jan 04 12:22:40 2016

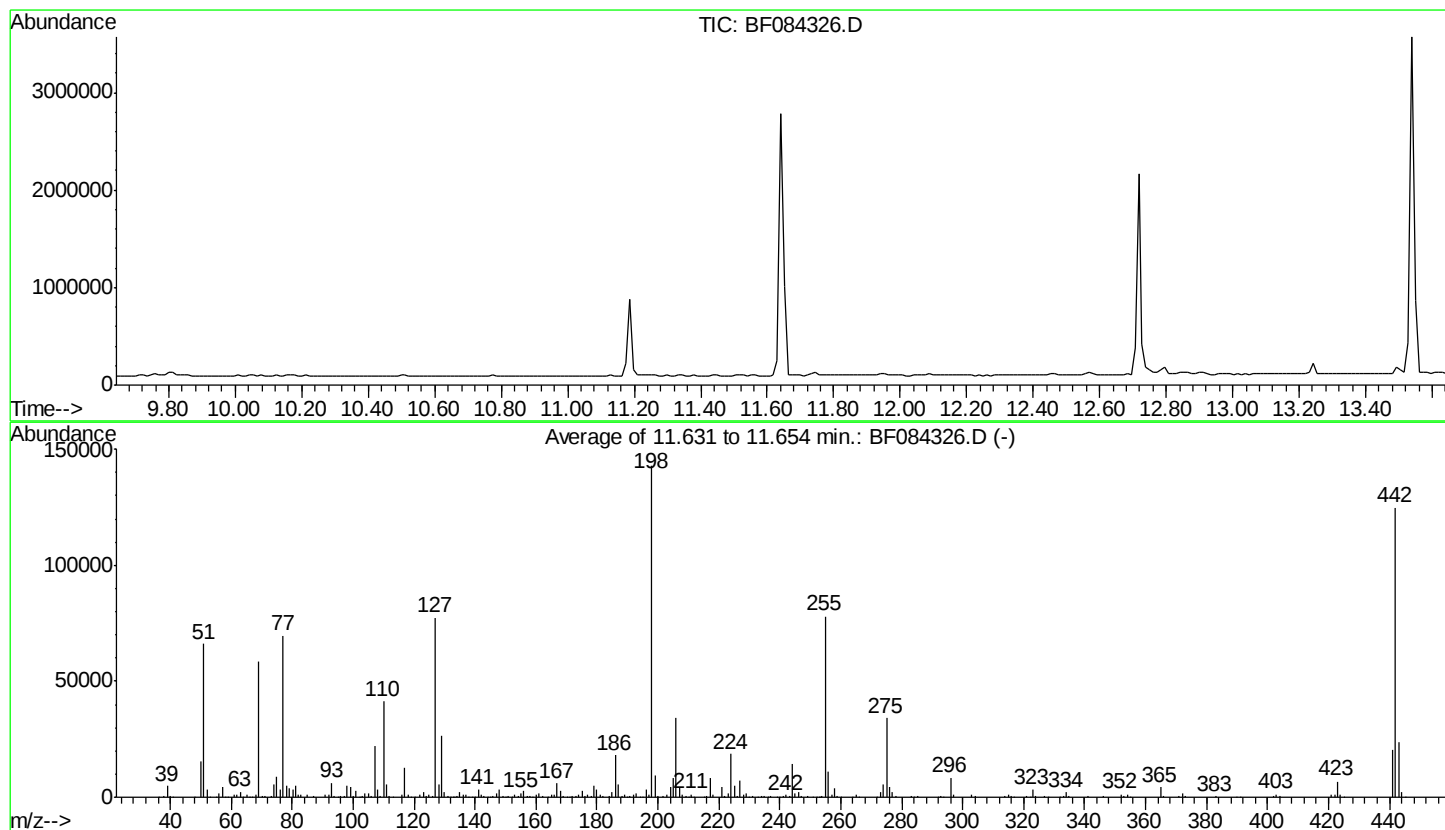

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	66041	PASS
68	69	0.00	2	1.7	1015	PASS
69	198	0.00	100	40.8	58299	PASS
70	69	0.00	2	0.8	454	PASS
127	198	10	80	54.2	77442	PASS
197	198	0.00	2	0.6	891	PASS
198	198	100	100	100.0	142942	PASS
199	198	5	9	6.6	9375	PASS
275	198	10	60	23.8	34009	PASS
365	198	1	100	3.1	4409	PASS
441	442	0.01	24	16.3	20304	PASS
442	198	50	100	87.4	124870	PASS
443	442	15	24	19.0	23696	PASS