


Data Path : Z:\HPCHEM1\BNA F\Data\BF010816\
 Data File : BF084340.D
 Acq On : 8 Jan 2016 21:35
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

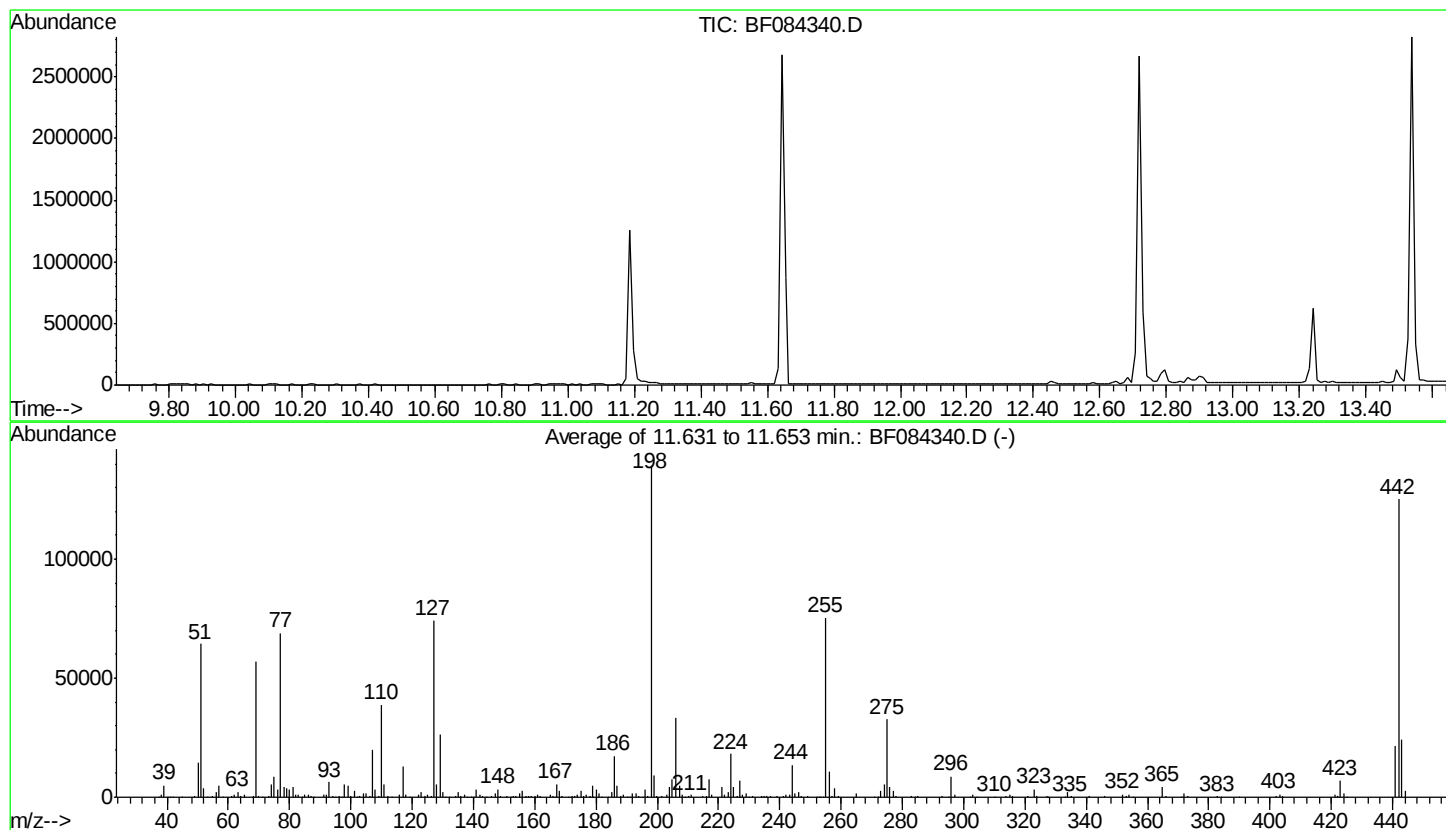

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	64438	PASS
68	69	0.00	2	1.4	813	PASS
69	198	0.00	100	40.7	56731	PASS
70	69	0.00	2	0.7	400	PASS
127	198	10	80	53.2	74021	PASS
197	198	0.00	2	0.6	786	PASS
198	198	100	100	100.0	139226	PASS
199	198	5	9	6.7	9352	PASS
275	198	10	60	23.4	32582	PASS
365	198	1	100	3.1	4359	PASS
441	442	0.01	24	17.0	21294	PASS
442	198	50	100	89.9	125123	PASS
443	442	15	24	19.1	23949	PASS