


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF010820\
 Data File : BF118494.D
 Acq On : 8 Jan 2020 11:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 16:06:11 2020

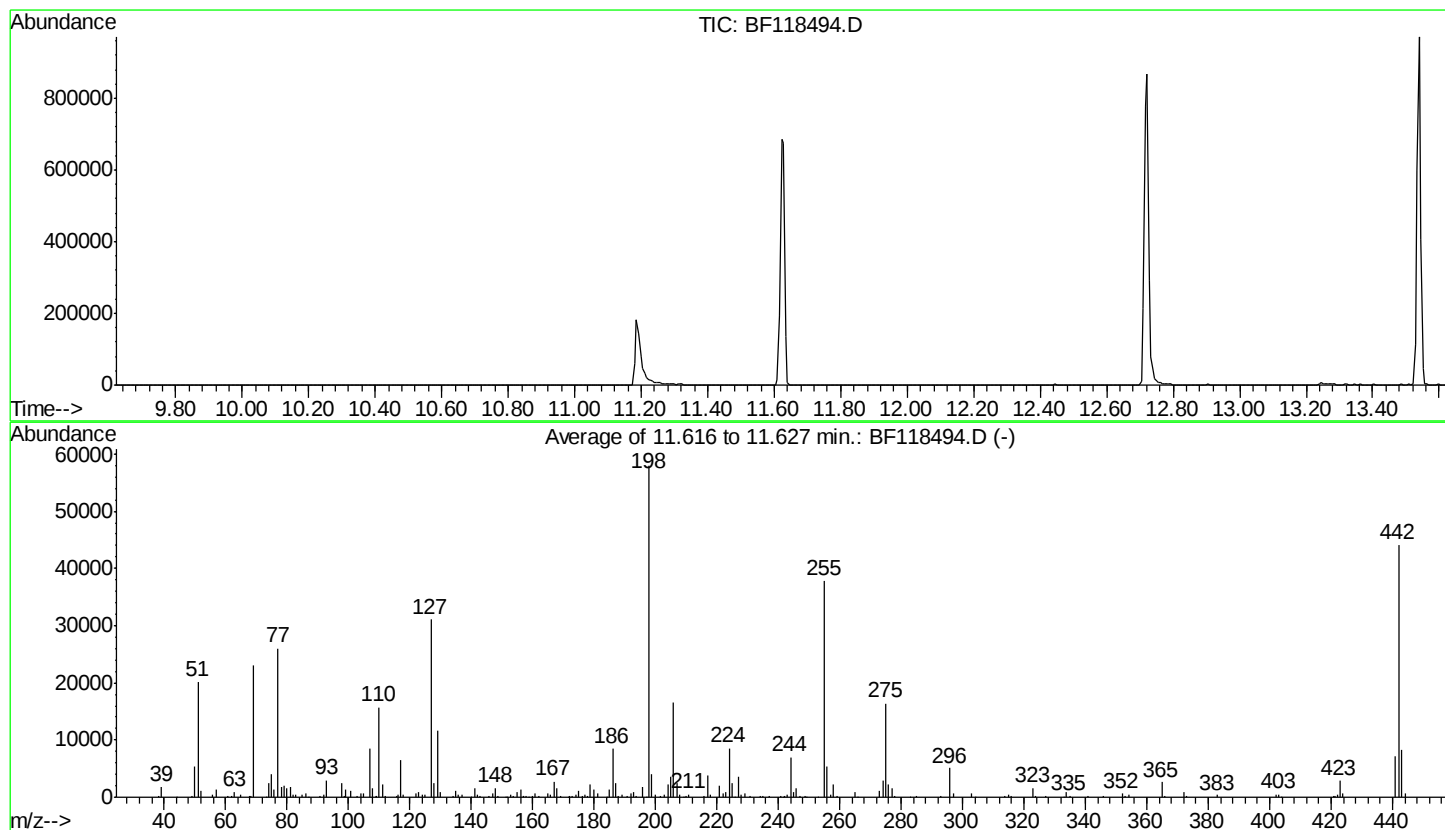

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	20199	PASS
68	69	0.00	2	1.3	295	PASS
69	198	0.00	100	39.8	23082	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	31014	PASS
197	198	0.00	2	0.2	108	PASS
198	198	100	100	100.0	57968	PASS
199	198	5	9	6.8	3926	PASS
275	198	10	60	28.4	16447	PASS
365	198	1	100	4.5	2586	PASS
441	198	0.01	100	12.4	7210	PASS
442	198	50	100	76.1	44137	PASS
443	442	15	24	18.9	8332	PASS