
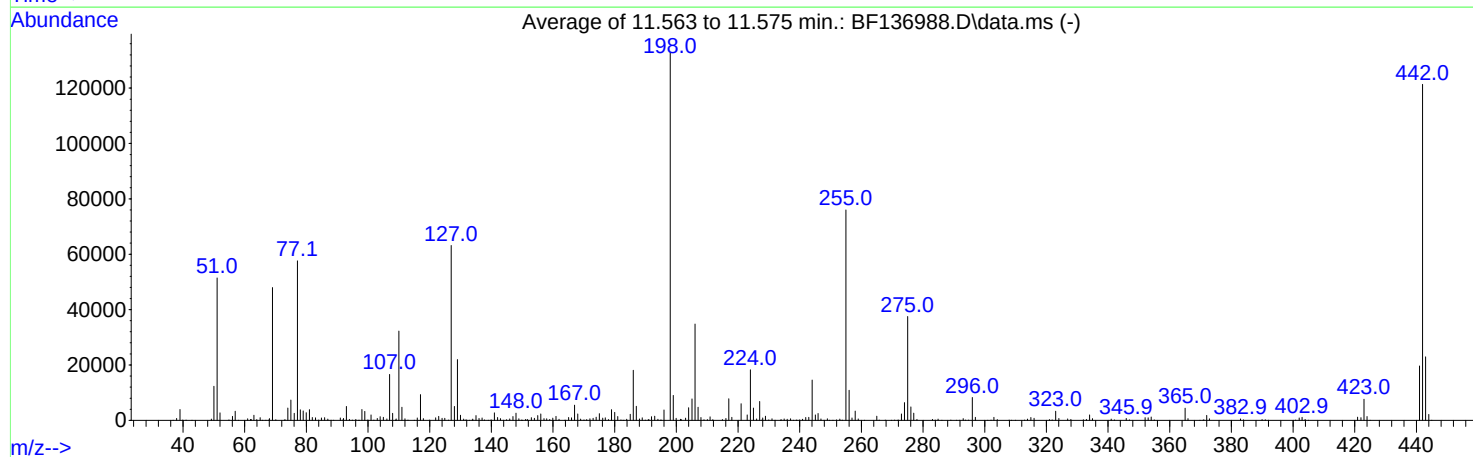


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010824\
Data File : BF136988.D
Acq On : 08 Jan 2024 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

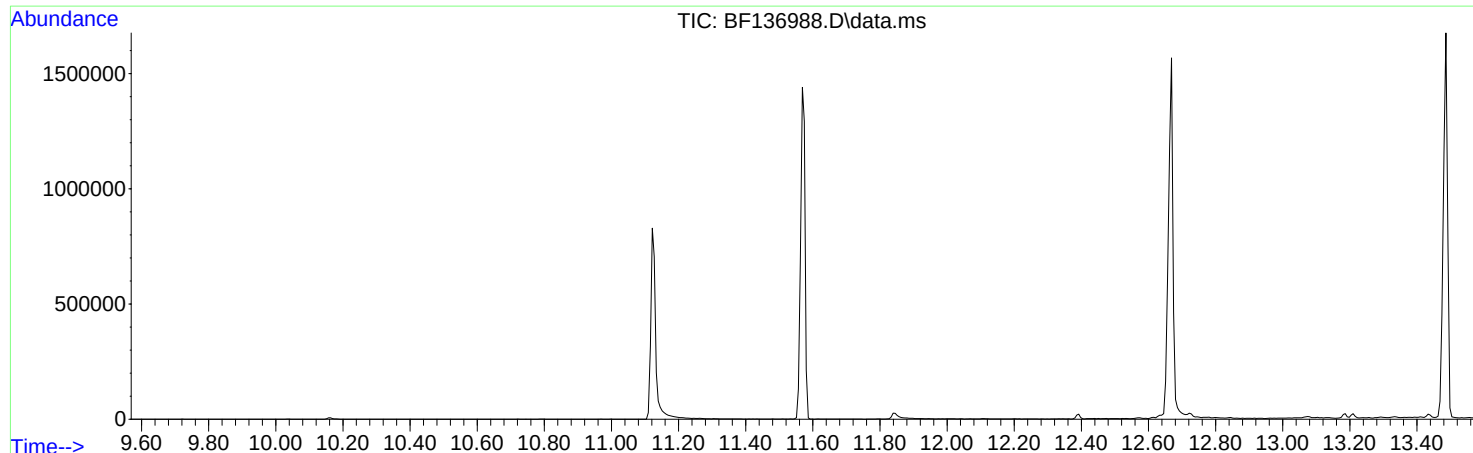




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	51459	PASS
68	69	0.00	2	1.3	633	PASS
69	198	0.00	100	36.1	47973	PASS
70	69	0.00	2	0.4	211	PASS
127	198	10	80	47.5	63160	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	132848	PASS
199	198	5	9	6.8	9006	PASS
275	198	10	60	28.2	37525	PASS
365	198	1	100	3.3	4393	PASS
441	198	0.01	100	14.8	19624	PASS
442	442	50	100	100.0	121325	PASS
443	442	15	24	18.9	22949	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010824\
Data File : BF136988.D
Acq On : 08 Jan 2024 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 08 10:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

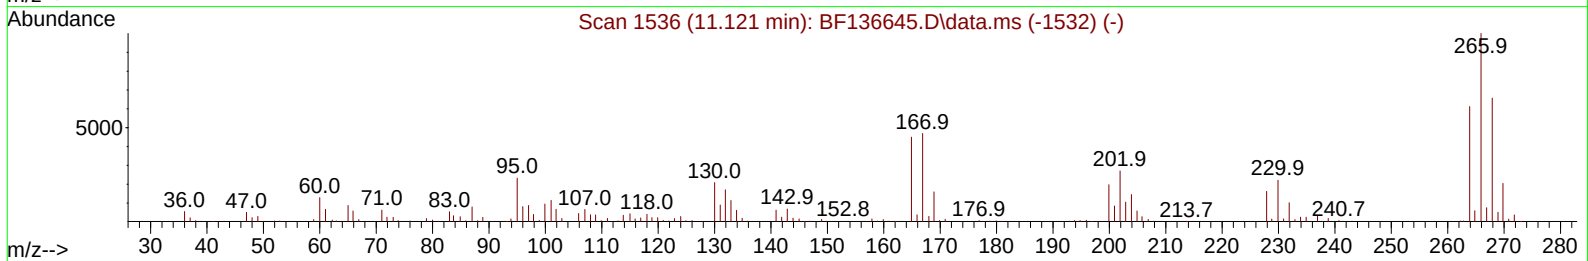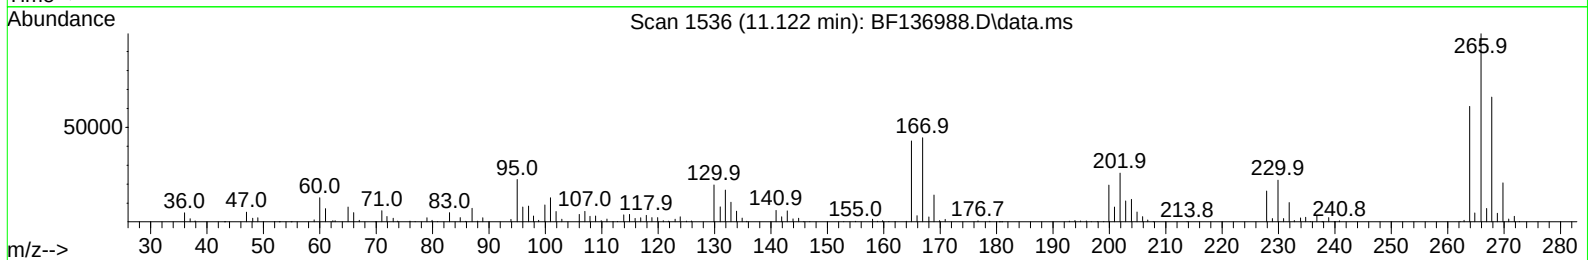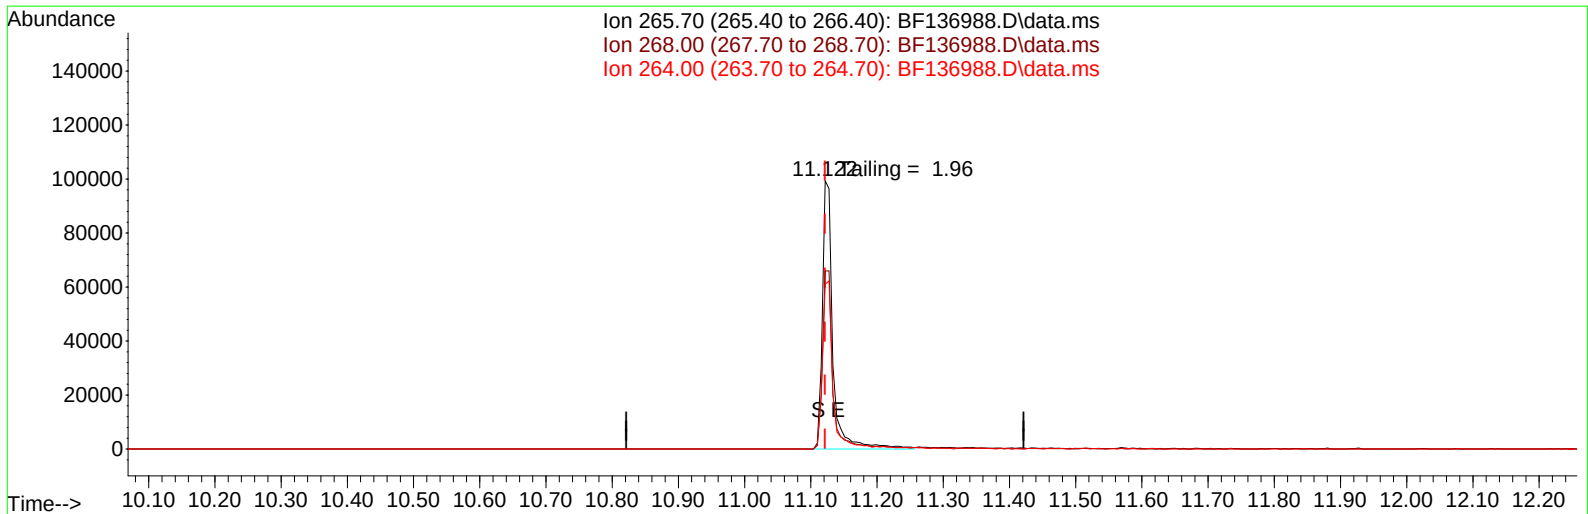

TIC: BF136988.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.000) 35040.76 ng




response 109561

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	66.33
264.00	61.20	61.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010824\
Data File : BF136988.D
Acq On : 08 Jan 2024 10:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 08 10:58:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

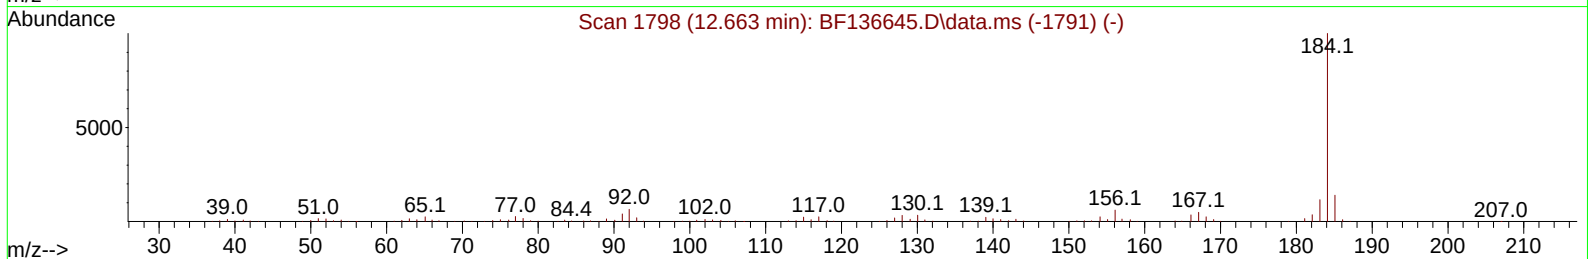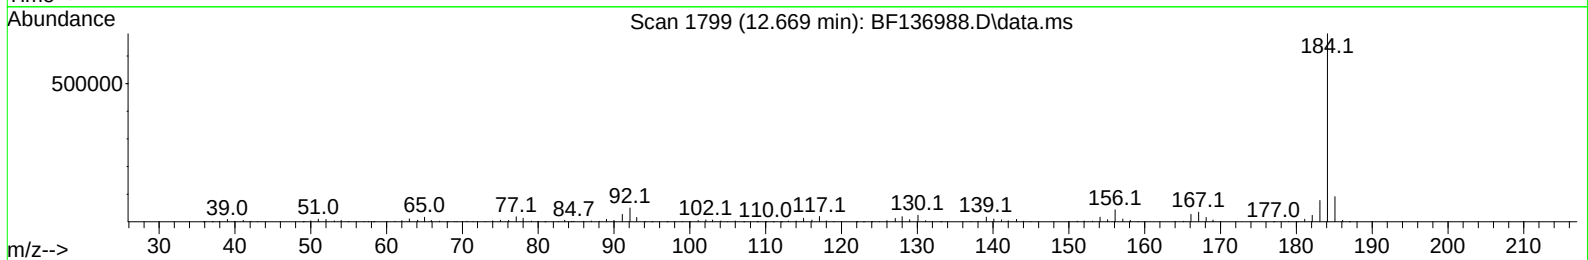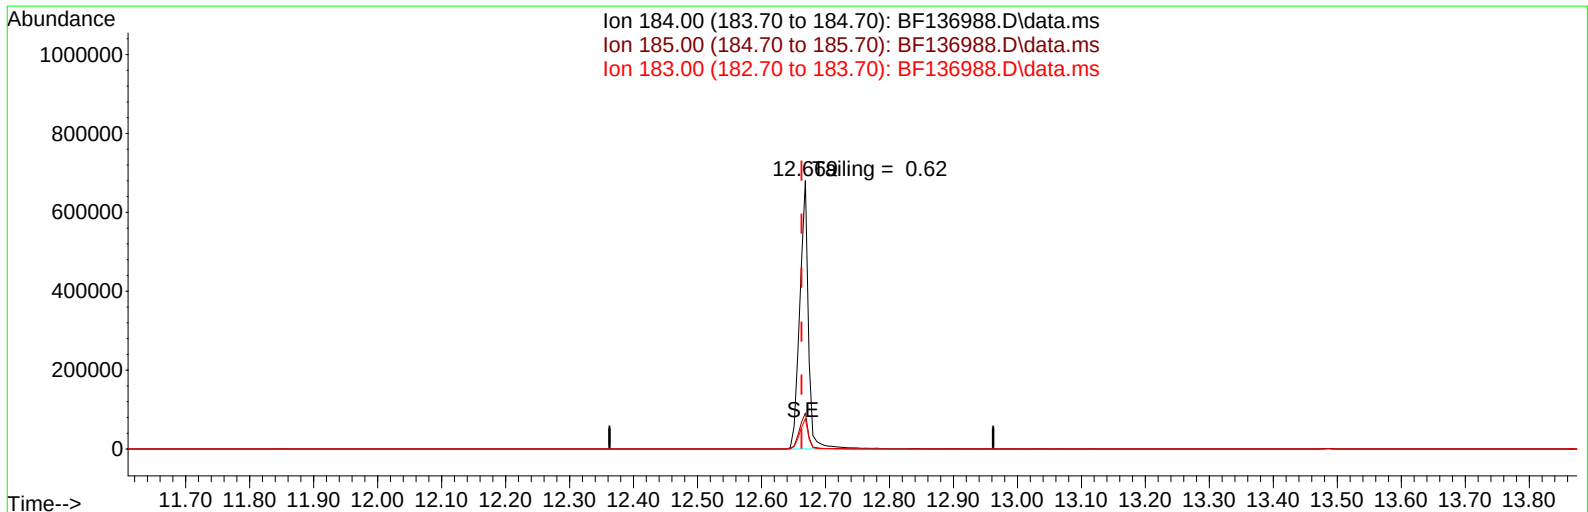

TIC: BF136988.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 0.00 ng

response 645383

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.42
183.00	11.60	11.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/8/2024	BNA_F	<u>BF136988.D</u>
Compound Name	Response	Retention Time
DDT	311870	13.486
DDD	7565	13.186
DDE	529	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8094	319964	2.53

Instrument :
BNA_F
ClientSampleId :
DFTPP