
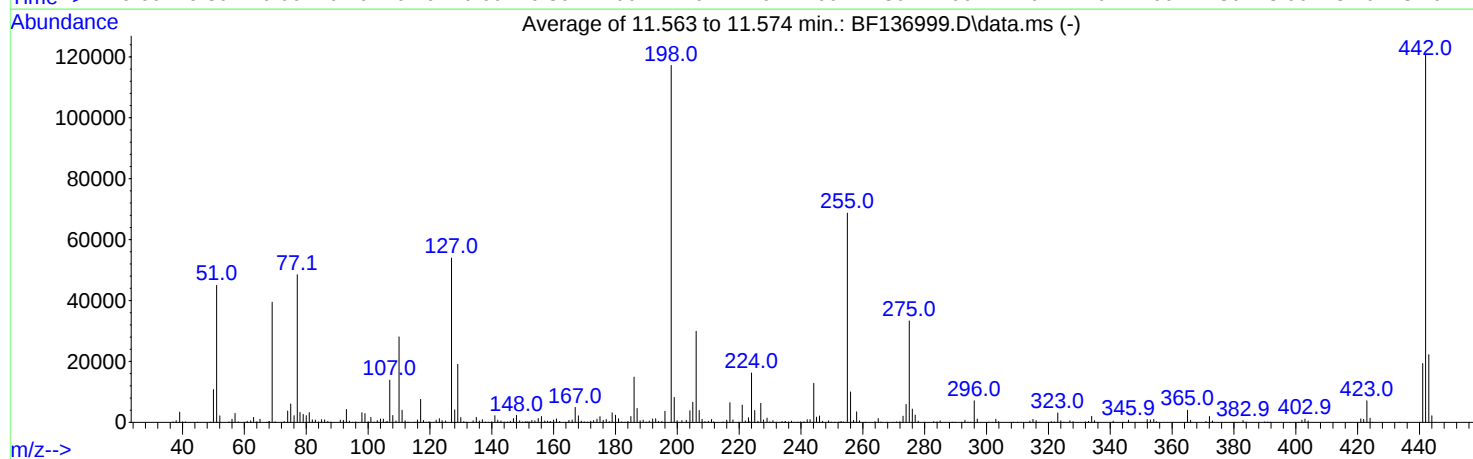


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010824\
Data File : BF136999.D
Acq On : 08 Jan 2024 16:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Dec 21 01:54:25 2023

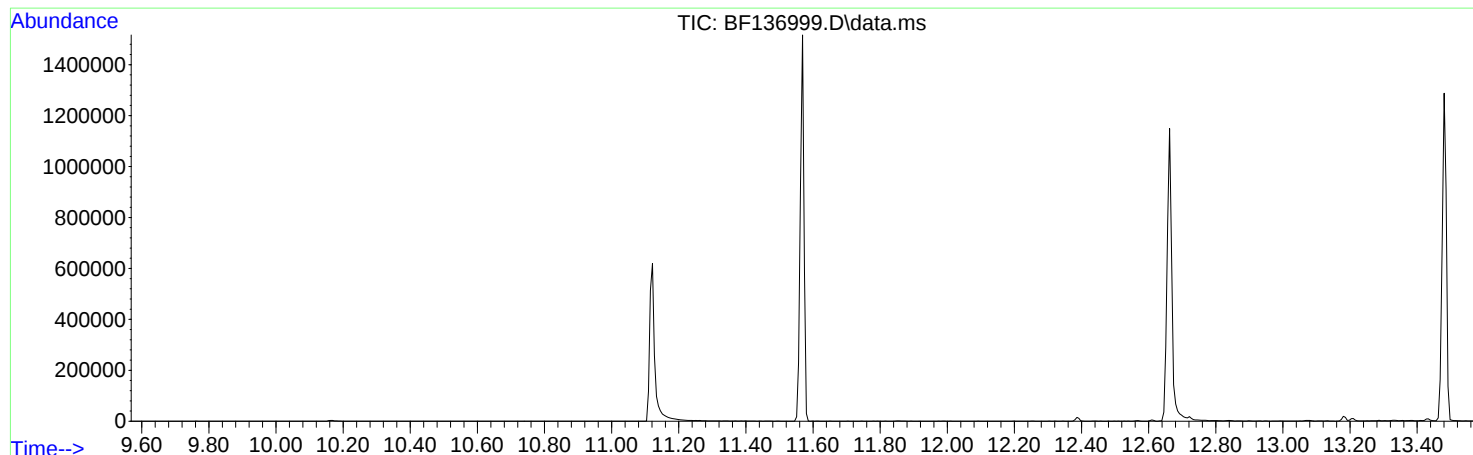




AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	44989	PASS
68	69	0.00	2	0.7	288	PASS
69	198	0.00	100	33.7	39462	PASS
70	69	0.00	2	0.5	211	PASS
127	198	10	80	46.0	53941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	117176	PASS
199	198	5	9	7.0	8220	PASS
275	198	10	60	28.4	33304	PASS
365	198	1	100	3.4	4007	PASS
441	198	0.01	100	16.5	19332	PASS
442	442	50	100	100.0	120773	PASS
443	442	15	24	18.4	22219	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010824\
Data File : BF136999.D
Acq On : 08 Jan 2024 16:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 08 17:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

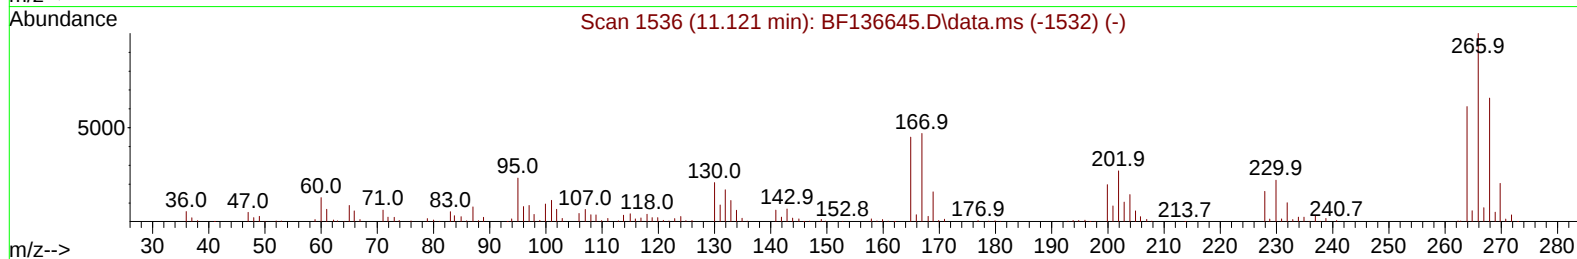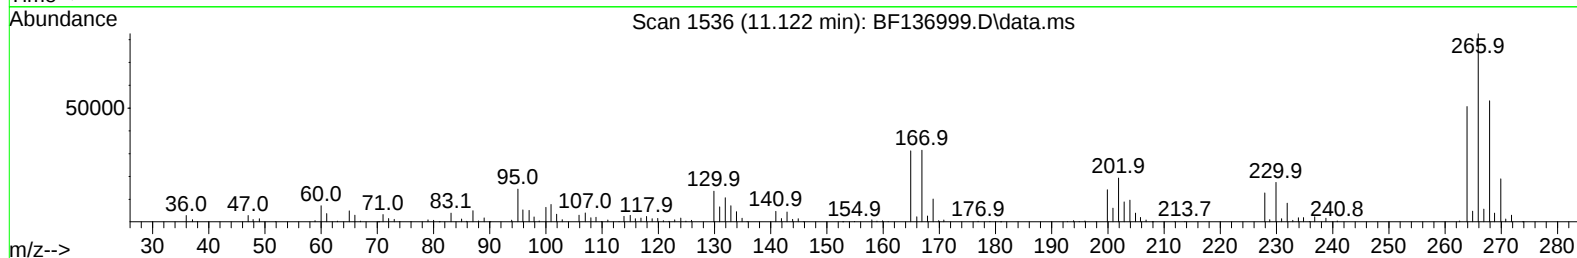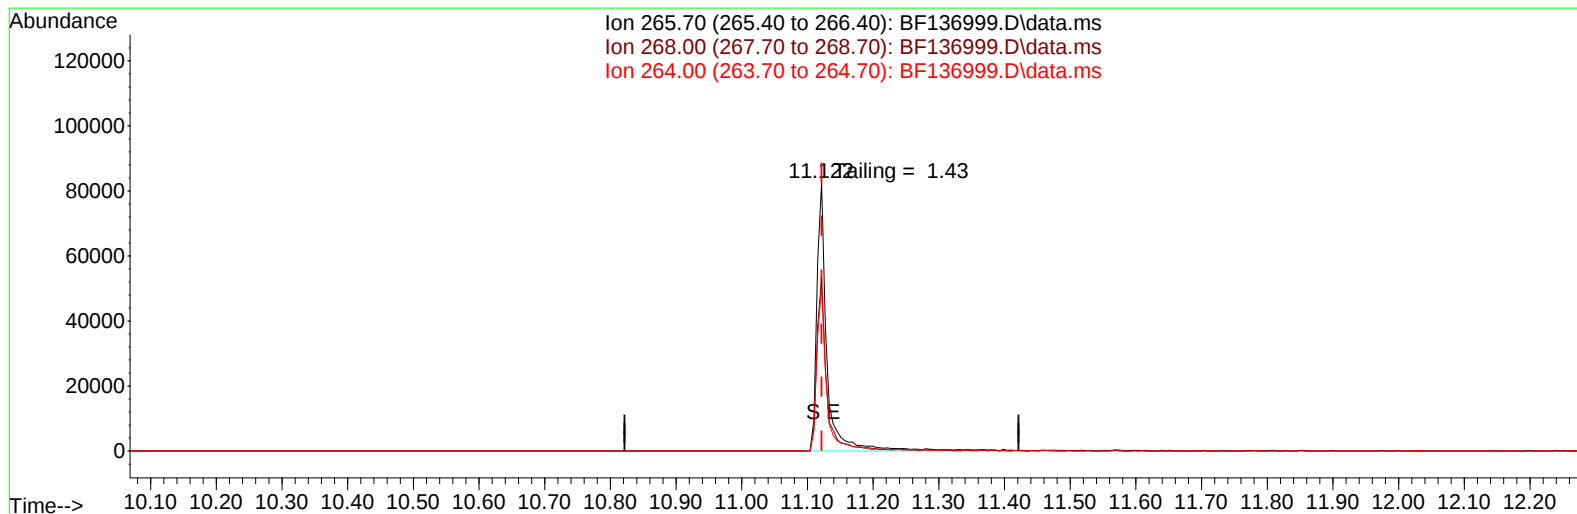

TIC: BF136999.D\data.ms

(70) Pentachlorophenol (C)

11.122min (+ 0.000) 27379.49 ng




response 87660

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	64.45
264.00	61.20	61.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010824\
Data File : BF136999.D
Acq On : 08 Jan 2024 16:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 08 17:14:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

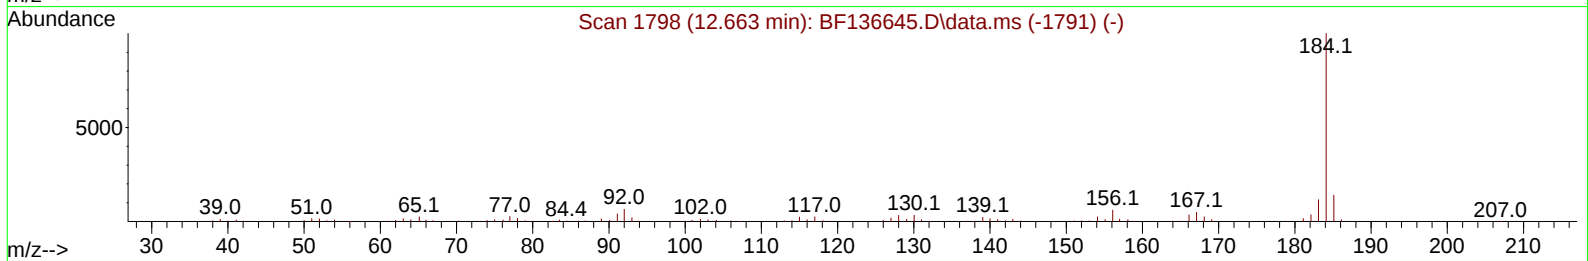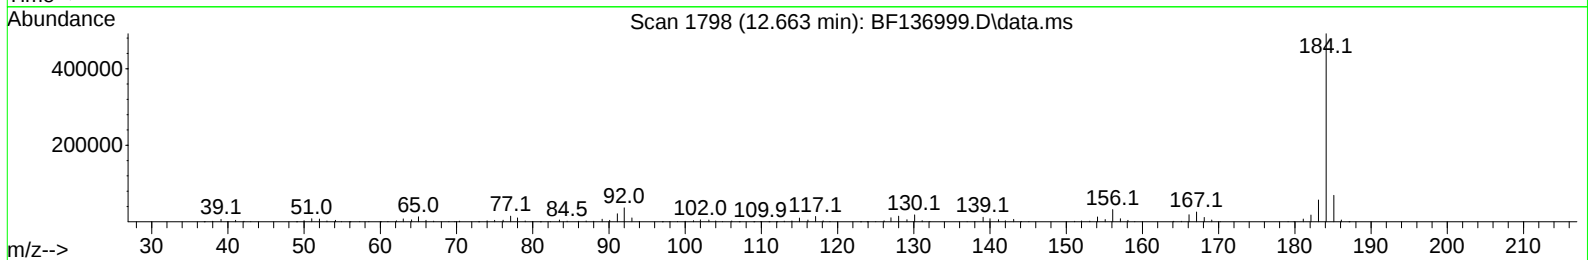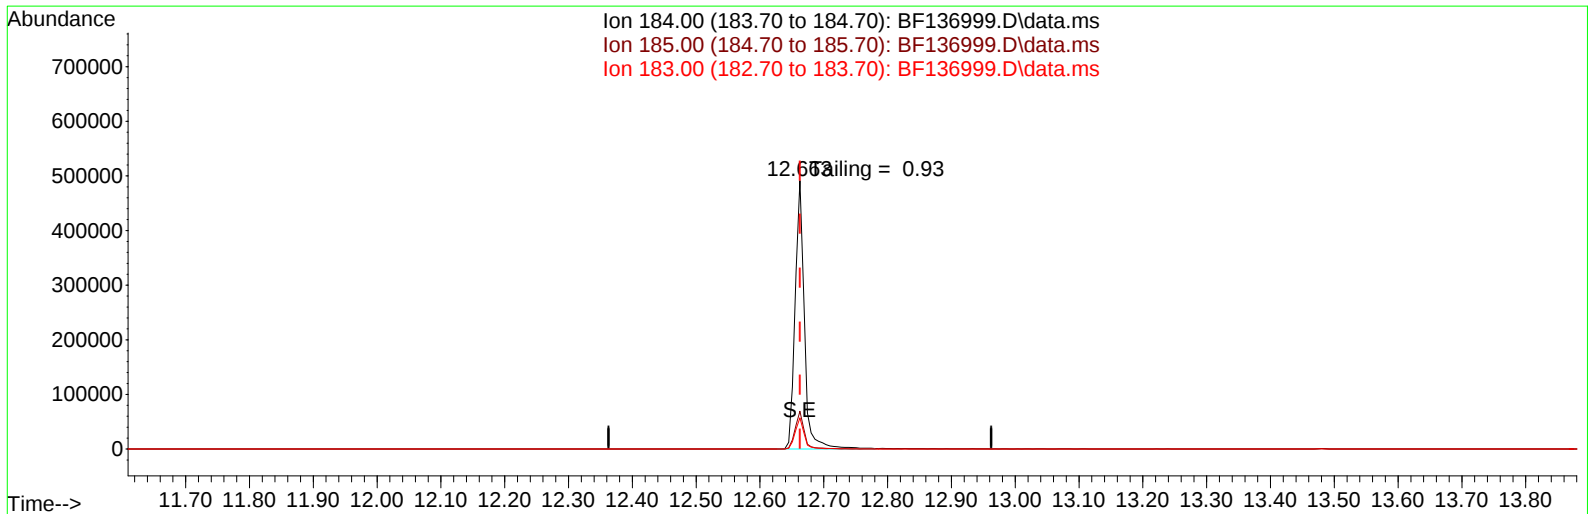

TIC: BF136999.D\data.ms

(77) Benzidine

12.663min (+ 0.000) 0.00 ng

response 504128

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.11
183.00	11.60	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/8/2024	BNA_F	<u>BF136999.D</u>
Compound Name	Response	Retention Time
DDT	240420	13.48
DDD	7024	13.18
DDE	504	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7528	247948	3.04

Instrument :
BNA_F
ClientSampleId :
DFTPP