
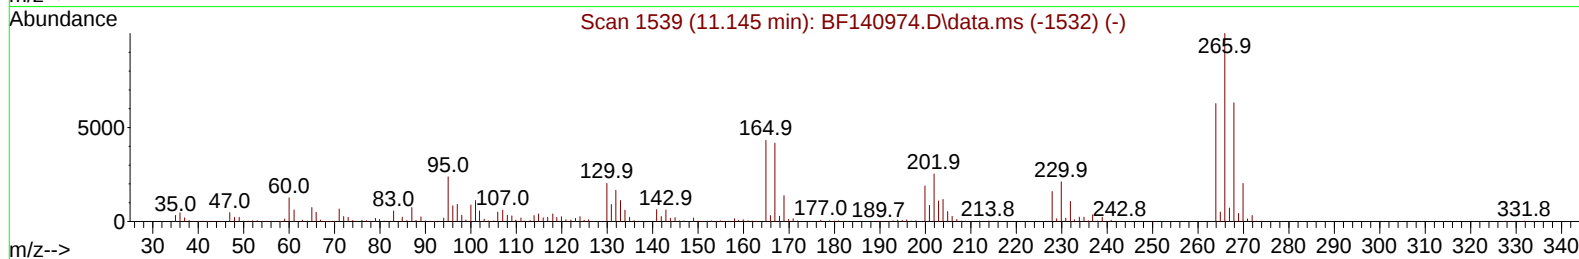
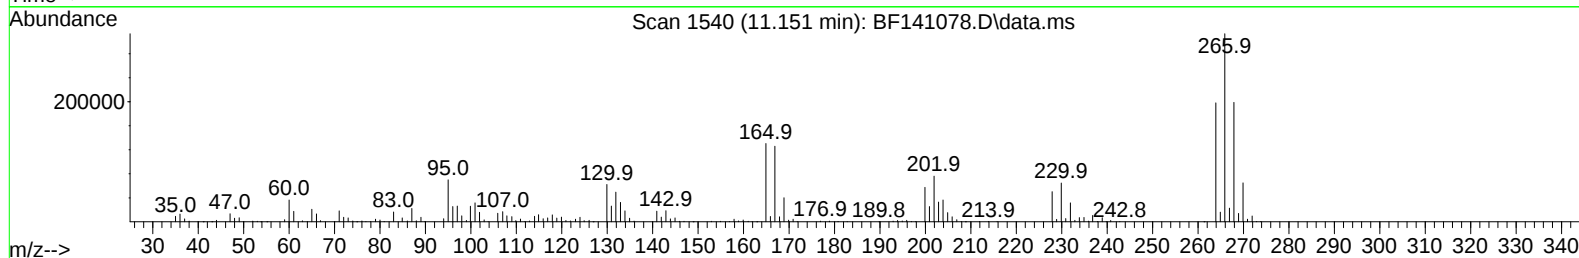


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010825\
Data File : BF141078.D
Acq On : 08 Jan 2025 10:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 08 11:07:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

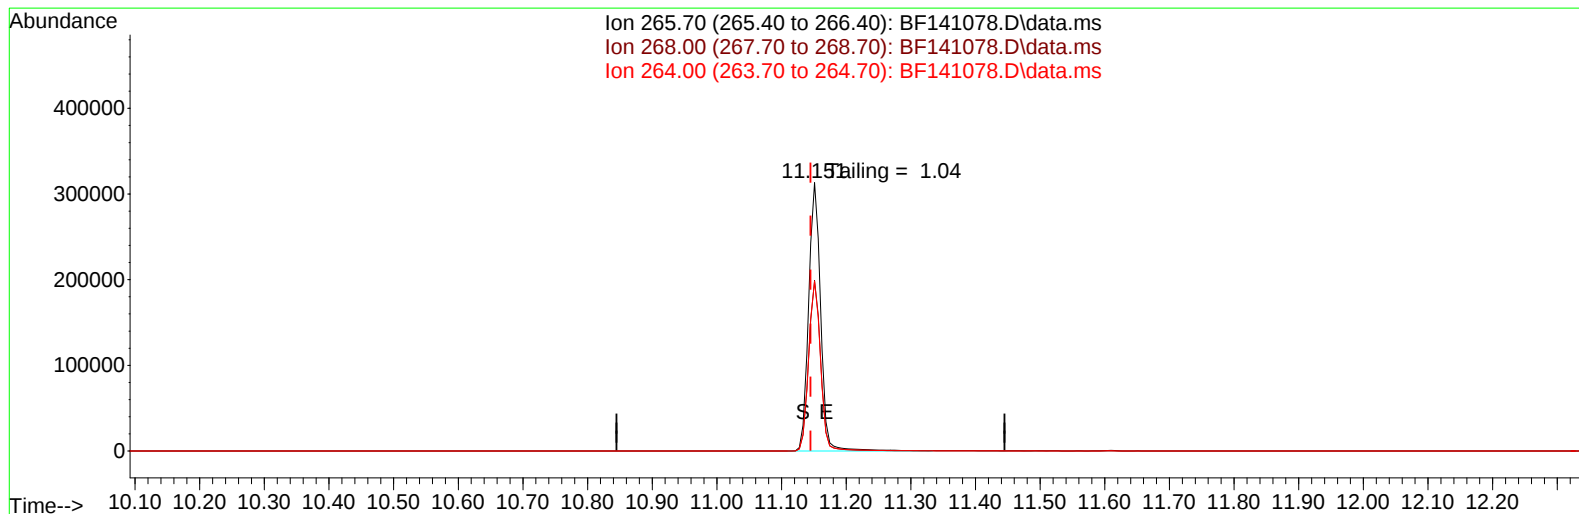

TIC: BF141078.D\data.ms

(70) Pentachlorophenol (C)




11.151min (+ 0.006) 82592.39 ng

response 407614

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.47
264.00	62.80	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010825\
Data File : BF141078.D
Acq On : 08 Jan 2025 10:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 08 11:07:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

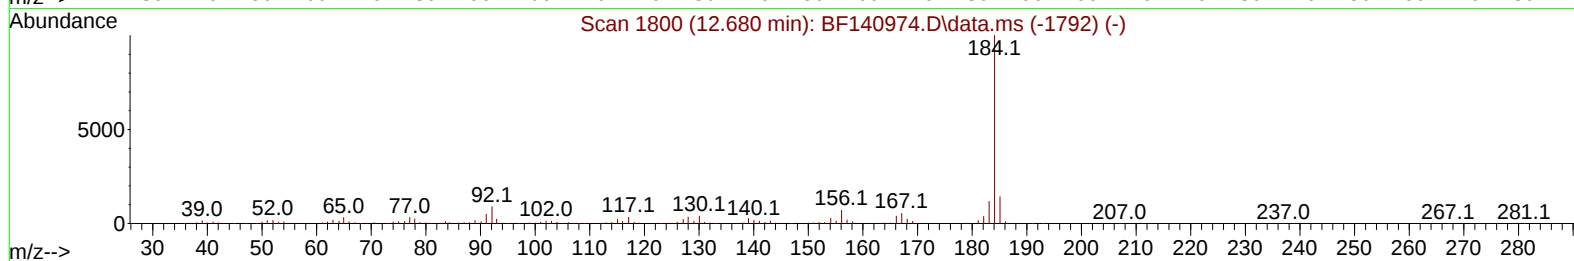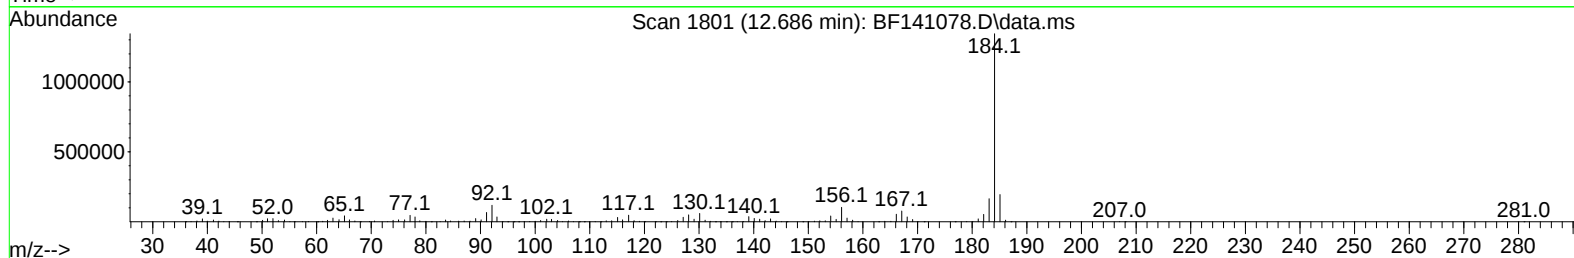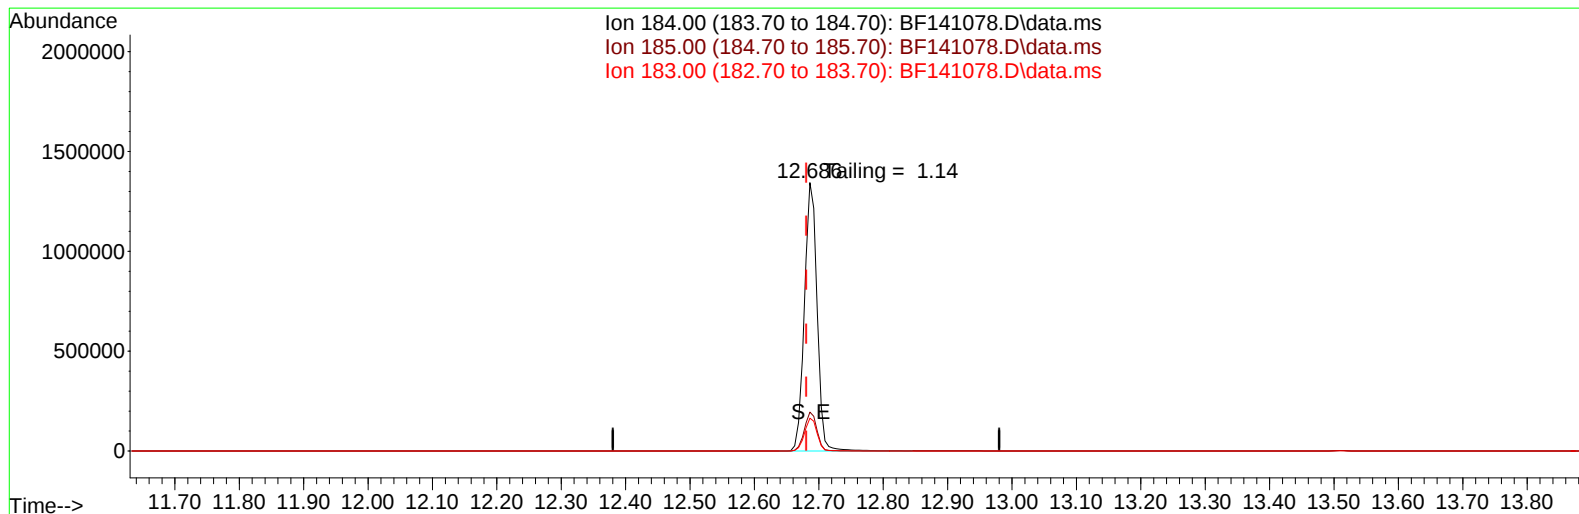

TIC: BF141078.D\data.ms

(77) Benzidine**12.686min (+ 0.006) 87528.11 ng****response 1846120**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.48
183.00	11.70	12.23
0.00	0.00	0.00