
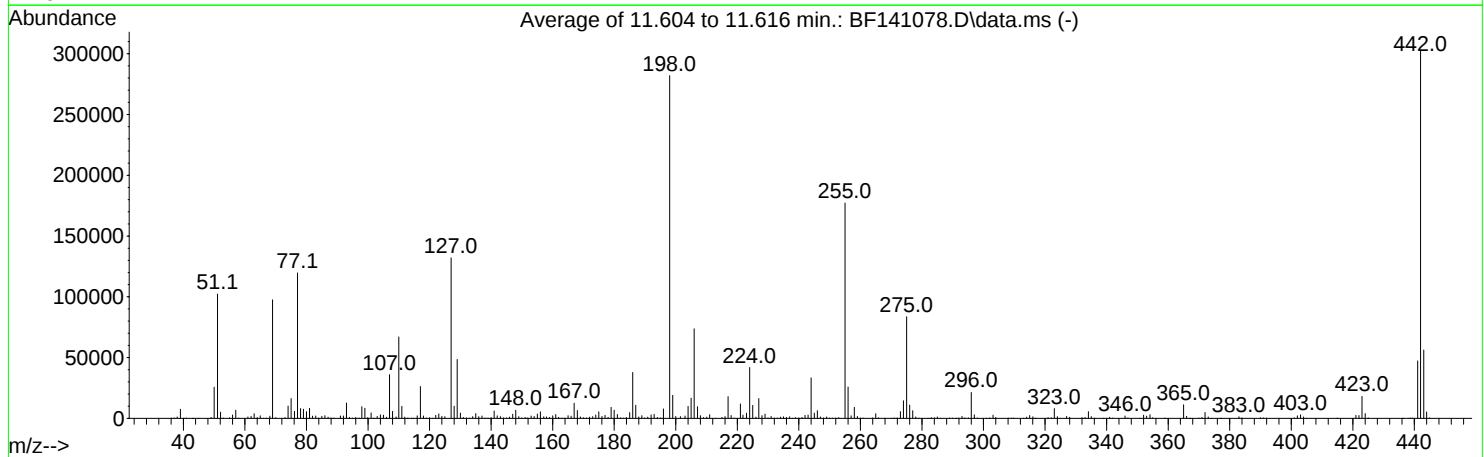


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010825\
Data File : BF141078.D
Acq On : 08 Jan 2025 10:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

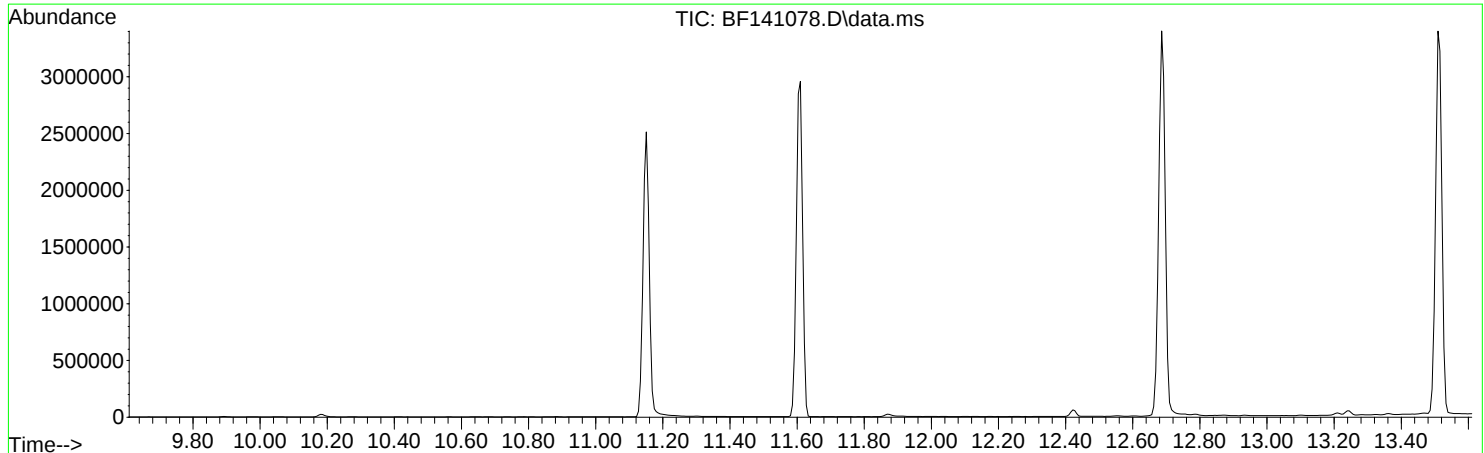

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	102328	PASS
68	69	0.00	2	1.9	1853	PASS
69	198	0.00	100	34.6	97621	PASS
70	69	0.00	2	0.6	592	PASS
127	198	10	80	46.9	132120	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	281984	PASS
199	198	5	9	6.7	18926	PASS
275	198	10	60	29.6	83608	PASS
365	198	1	100	3.9	11136	PASS
441	198	0.01	100	16.8	47288	PASS
442	442	50	100	100.0	302677	PASS
443	442	15	24	18.6	56285	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/8/2025	BNA_F	<u>BF141078.D</u>
Compound Name	Response	Retention Time
DDT	866235	13.51
DDD	13779	13.245
DDE	1022	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14801	881036	1.68

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010825\
Data File : BF141078.D
Acq On : 08 Jan 2025 10:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 08 11:07:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

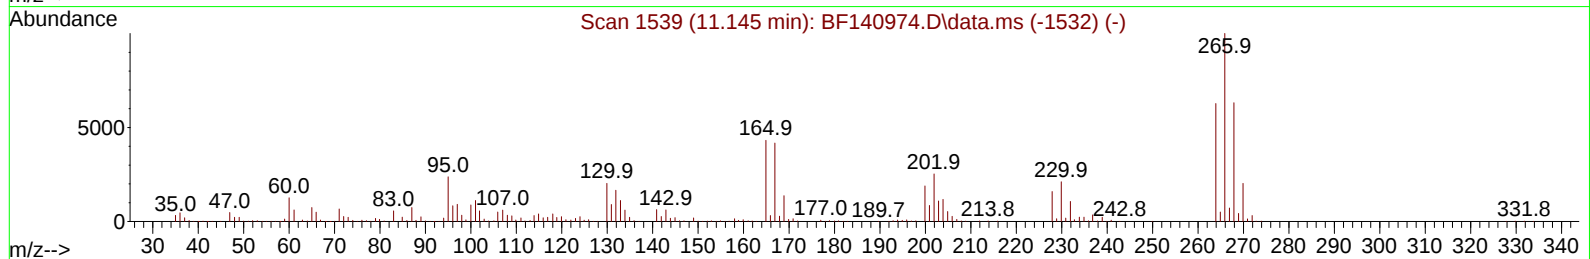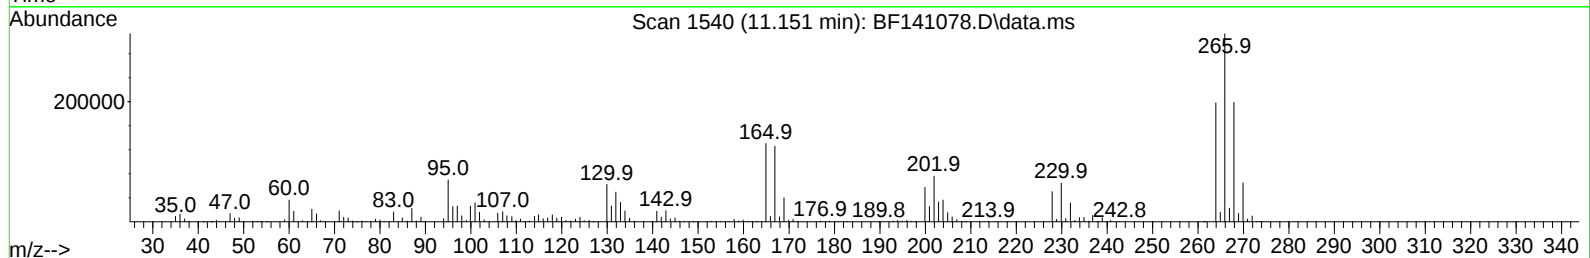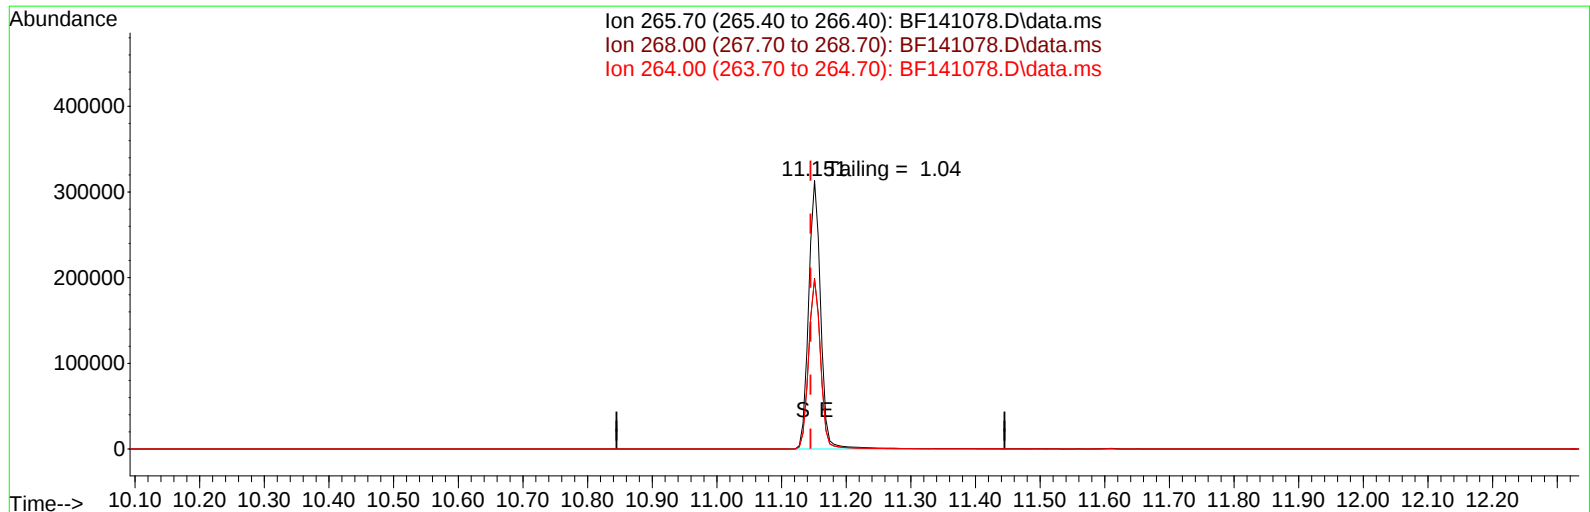

TIC: BF141078.D\data.ms

(70) Pentachlorophenol (C)

11.151min (+ 0.006) 82592.39 ng




response 407614

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.47
264.00	62.80	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010825\
Data File : BF141078.D
Acq On : 08 Jan 2025 10:23
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 08 11:07:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

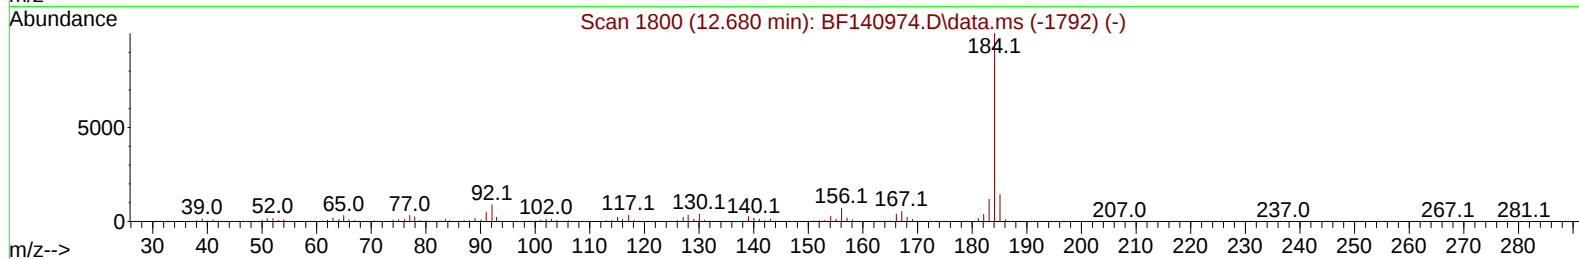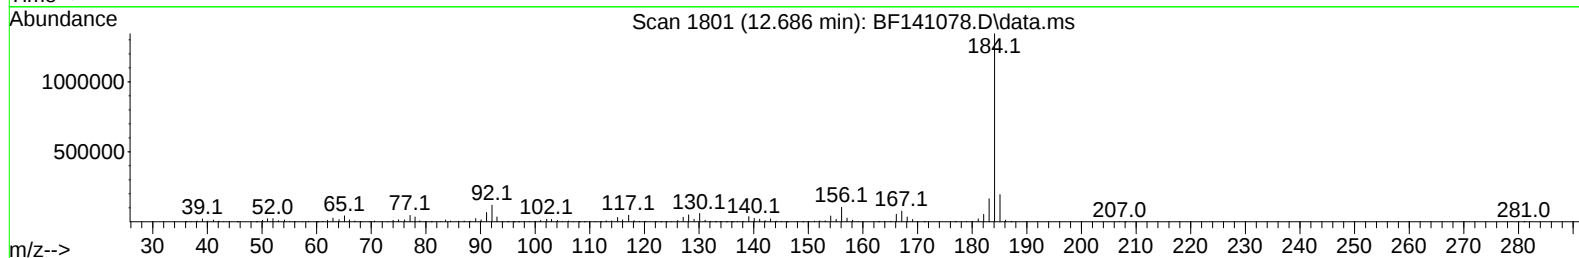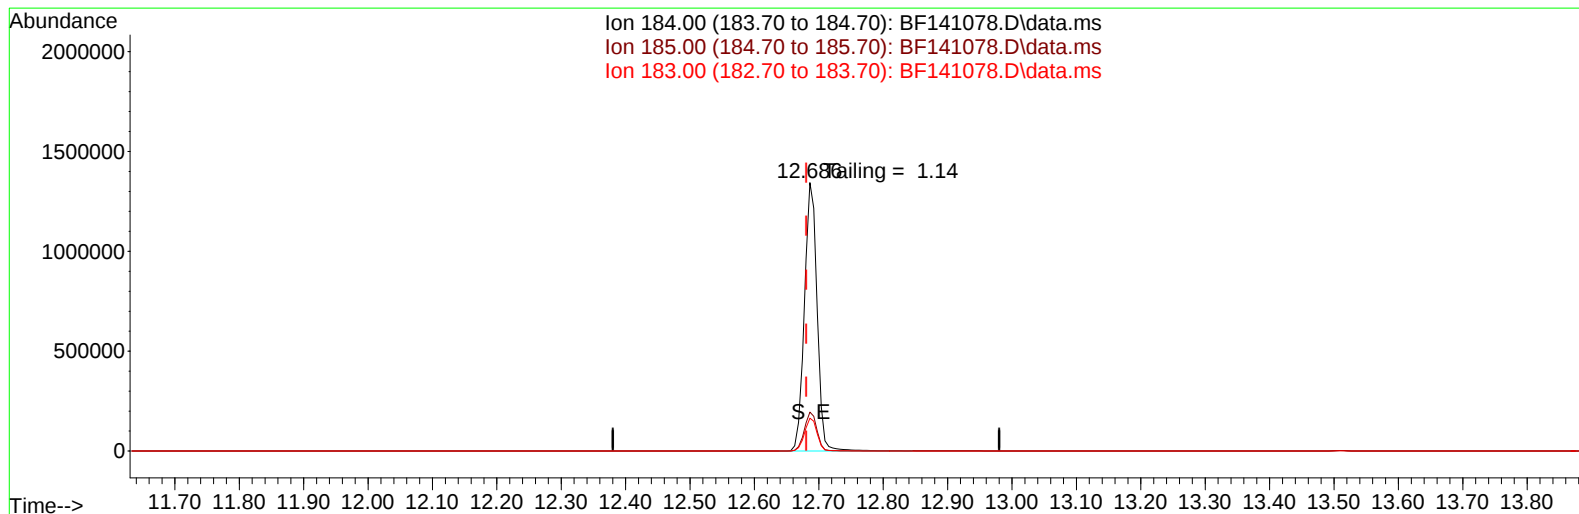

TIC: BF141078.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 87528.11 ng

response 1846120

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.48
183.00	11.70	12.23
0.00	0.00	0.00