


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010915\
 Data File : BF076788.D
 Acq On : 9 Jan 2015 15:47
 Operator : IZ / TP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 12 10:43:48 2015

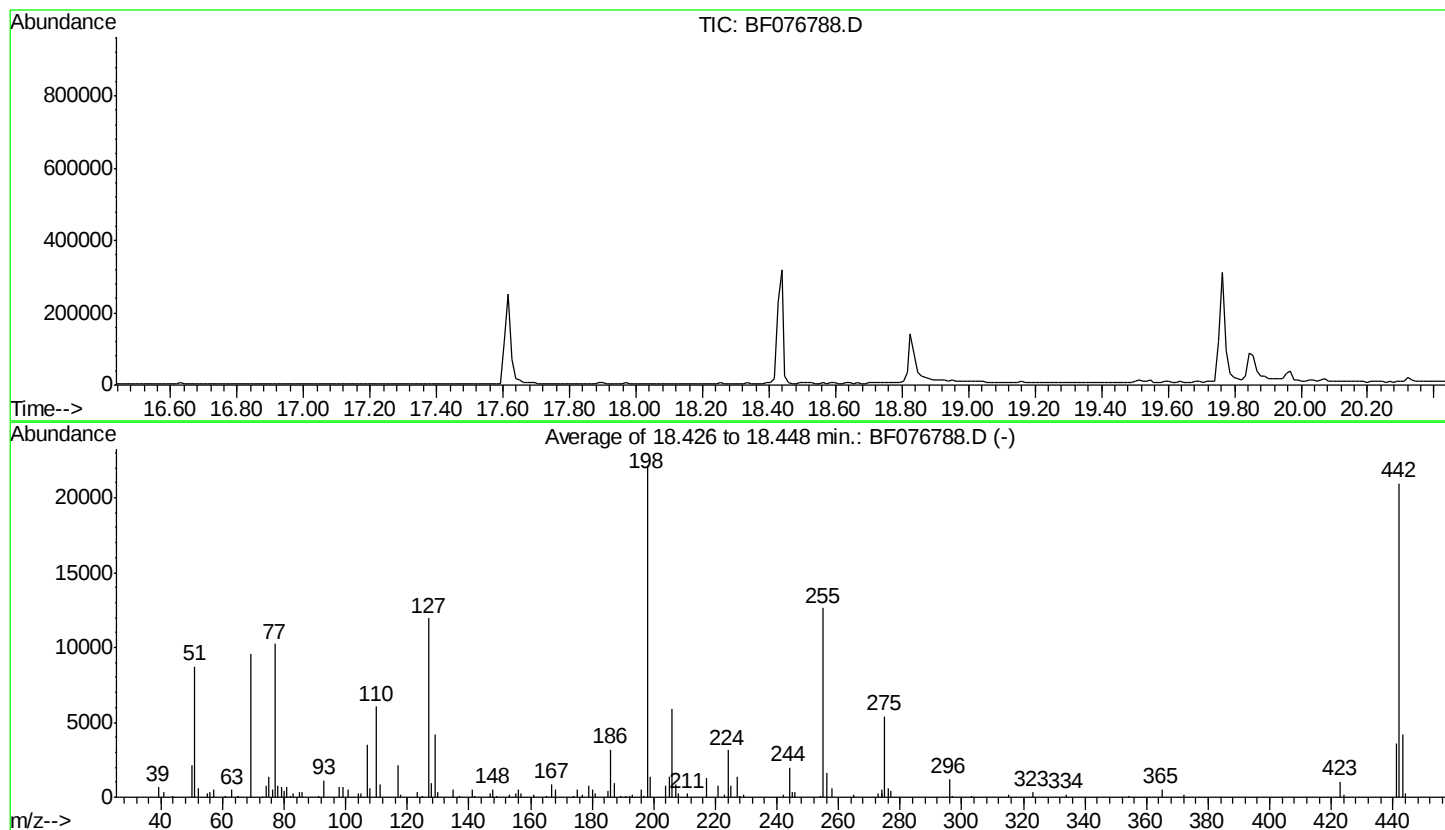

AutoFind: Scans 1517, 1518, 1519; Background Corrected with Scan 1513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	8734	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.4	9602	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.0	11965	PASS
197	198	0.00	2	0.5	113	PASS
198	198	100	100	100.0	22145	PASS
199	198	5	9	6.0	1331	PASS
275	198	10	60	24.5	5429	PASS
365	198	1	100	2.5	548	PASS
441	442	0.01	24	17.1	3582	PASS
442	198	50	100	94.7	20979	PASS
443	442	15	24	19.8	4159	PASS