
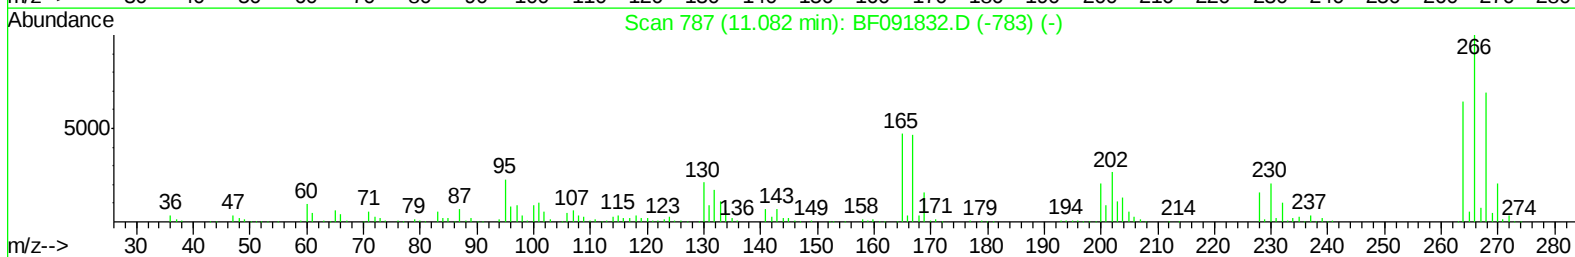
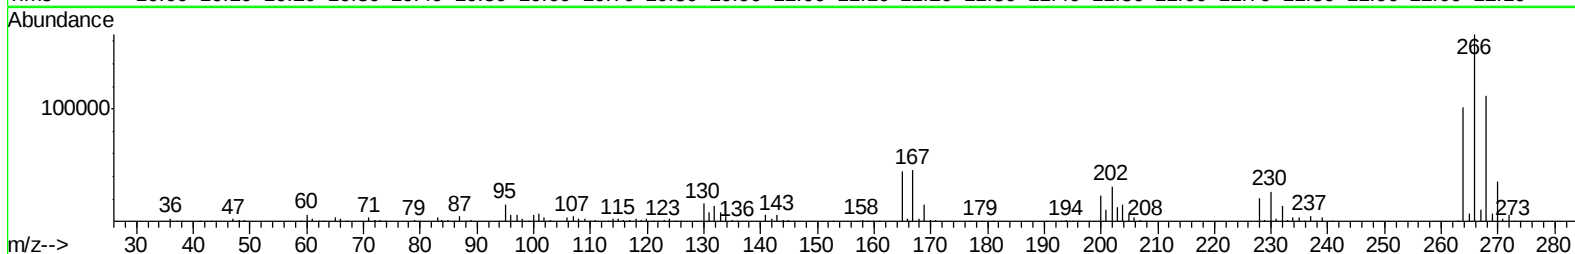


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010917\
Data File : BF092133.D
Acq On : 9 Jan 2017 12:15
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 07:47:40 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

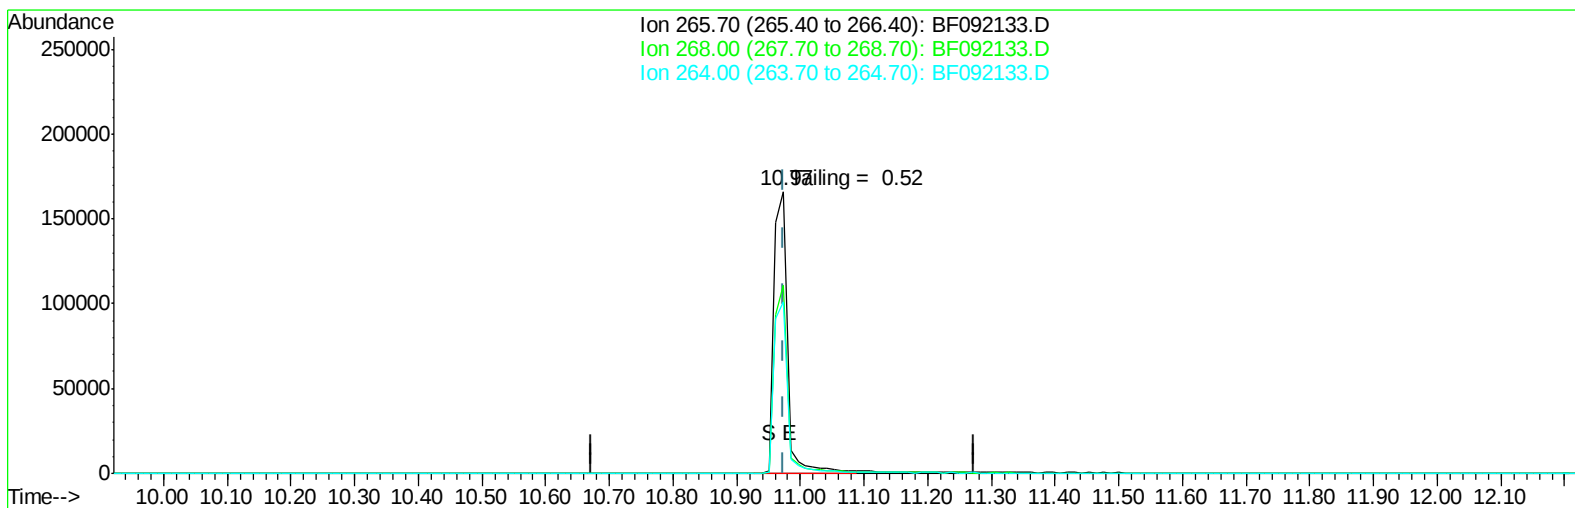

TIC: BF092133.D

(69) Pentachlorophenol (C)




10.973min (+0.000) 0.00ng

response 251942

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	66.99
264.00	62.90	60.83
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010917\  
Data File : BF092133.D  
Acq On    : 9 Jan 2017 12:15  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Jan 10 07:47:40 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

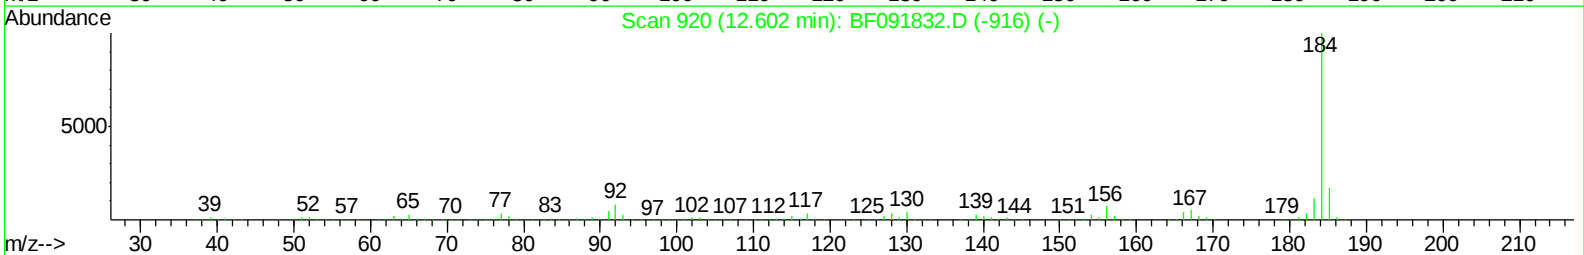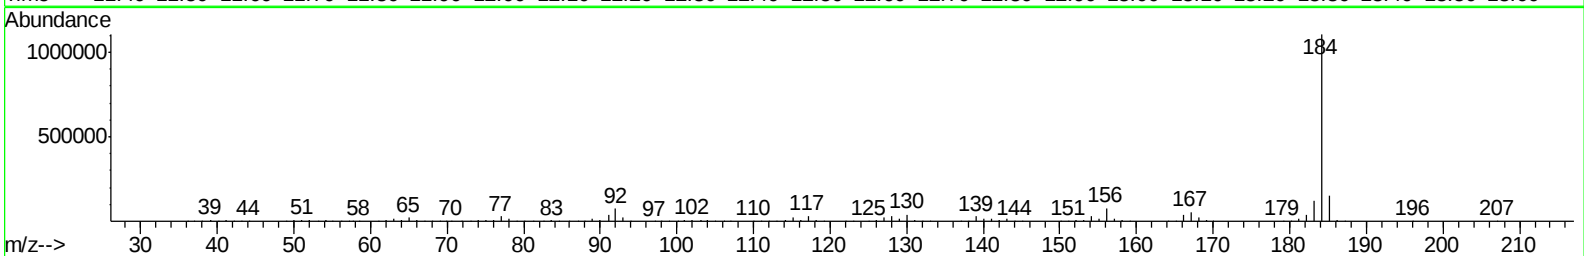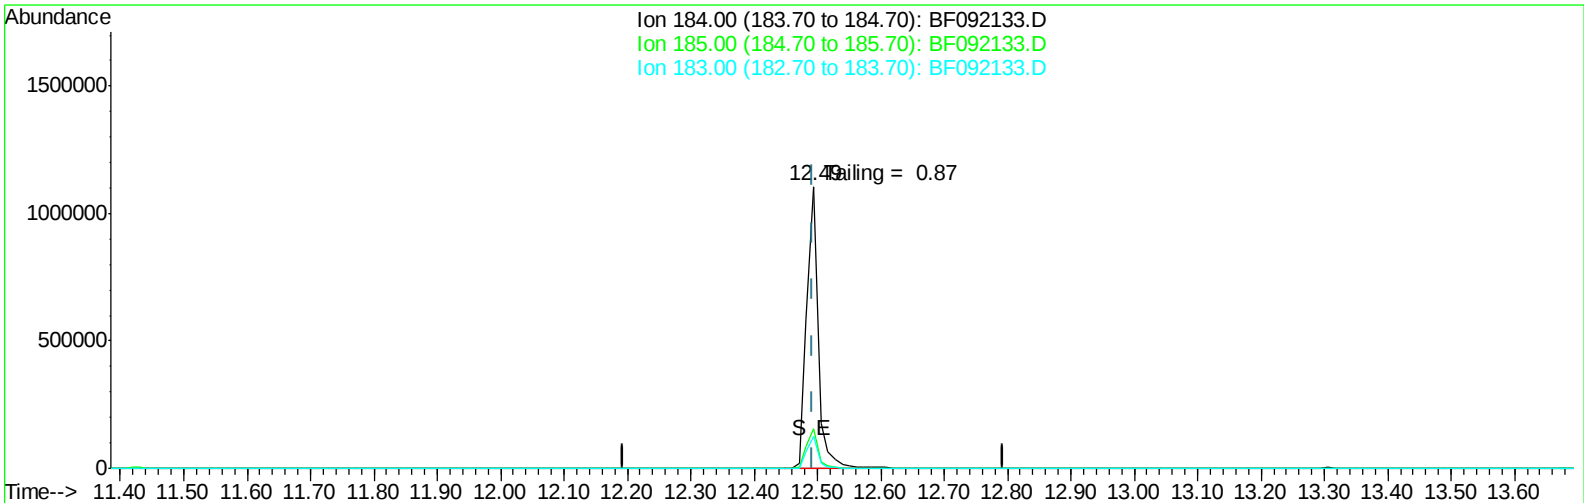

TIC: BF092133.D

(76) Benzidine

12.494min (+0.000) 0.00ng

response 1413725

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	13.97
183.00	11.50	11.28
0.00	0.00	0.00