
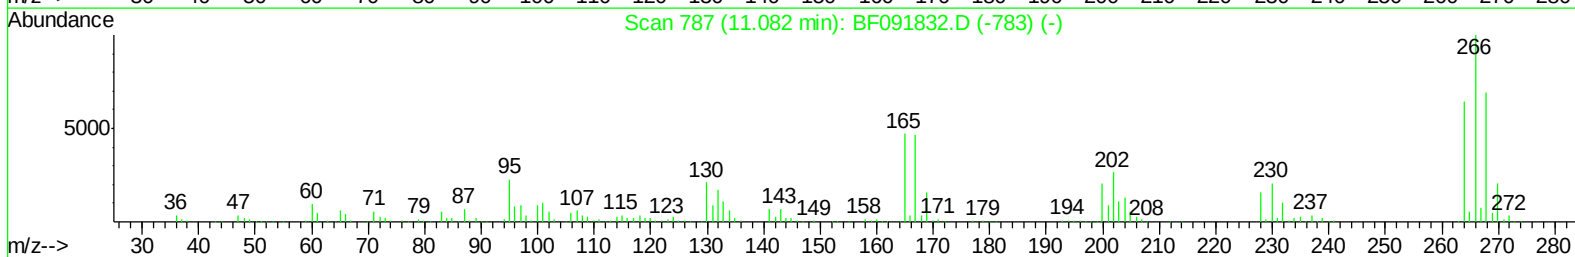
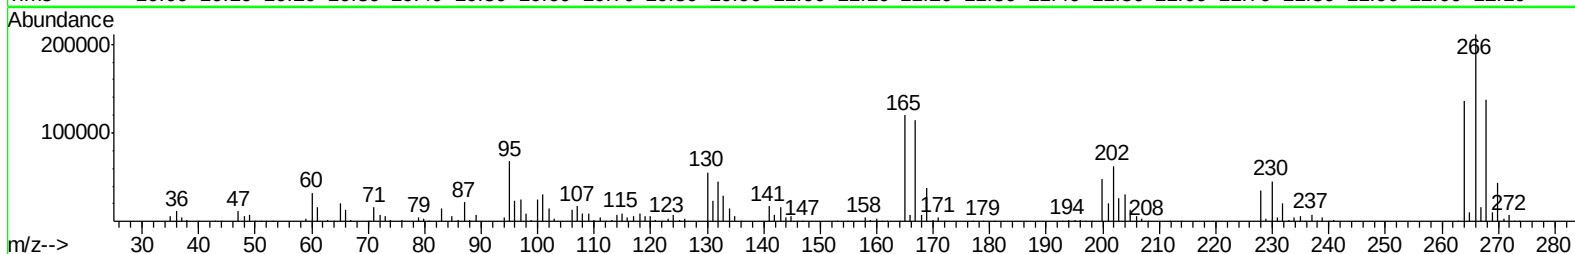


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010917\
Data File : BF092140.D
Acq On : 9 Jan 2017 15:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 07:48:20 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

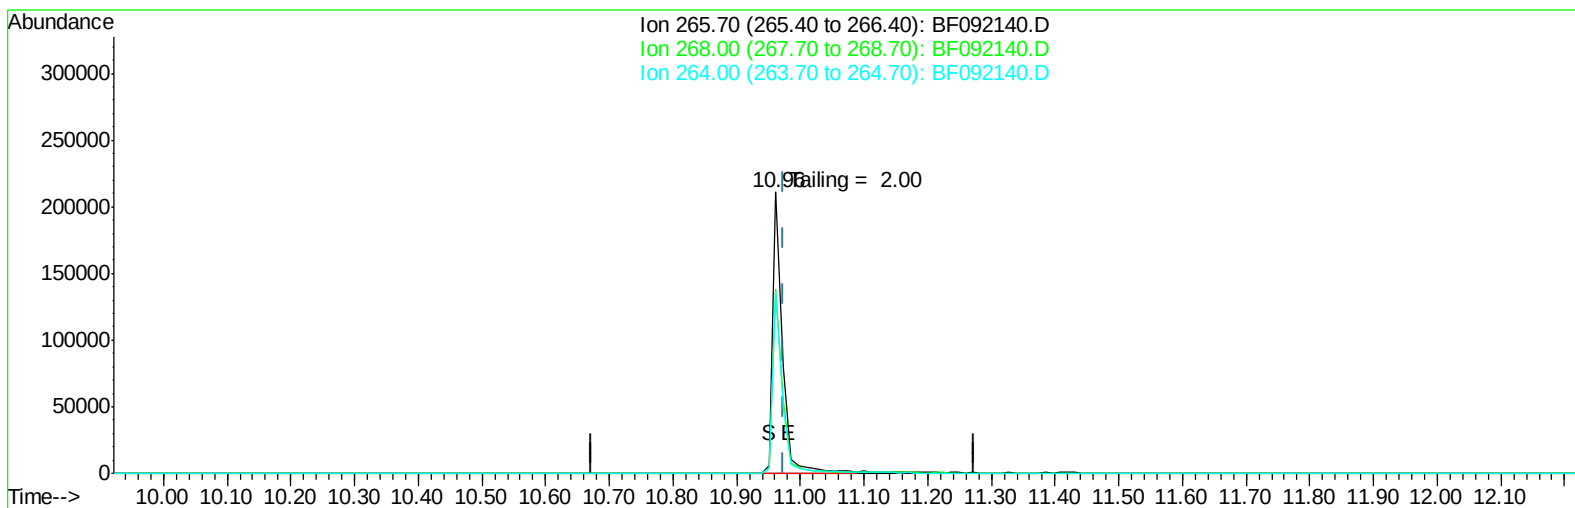

TIC: BF092140.D

(69) Pentachlorophenol (C)




10.962min (-0.011) 0.00ng

response 236464

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.42
264.00	62.90	64.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010917\
Data File : BF092140.D
Acq On : 9 Jan 2017 15:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 07:48:20 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

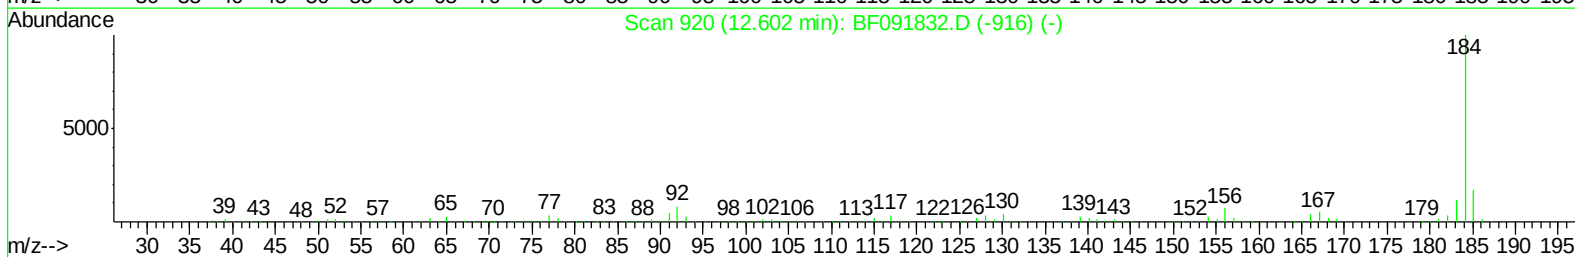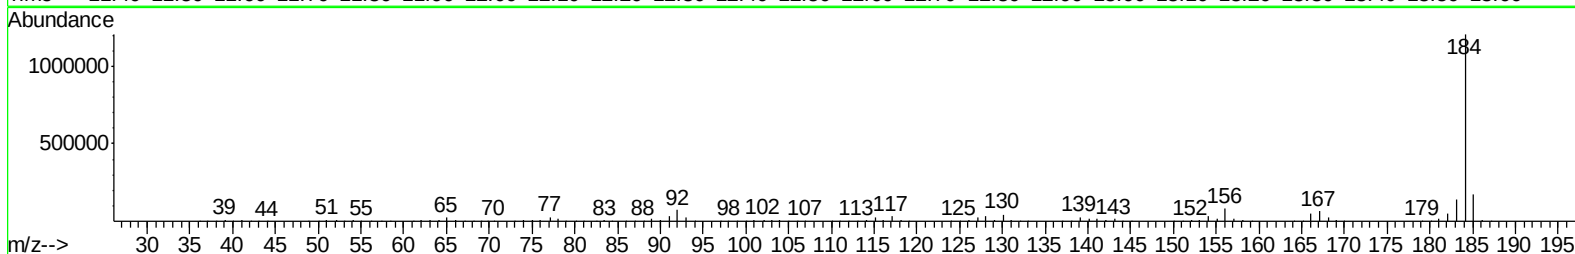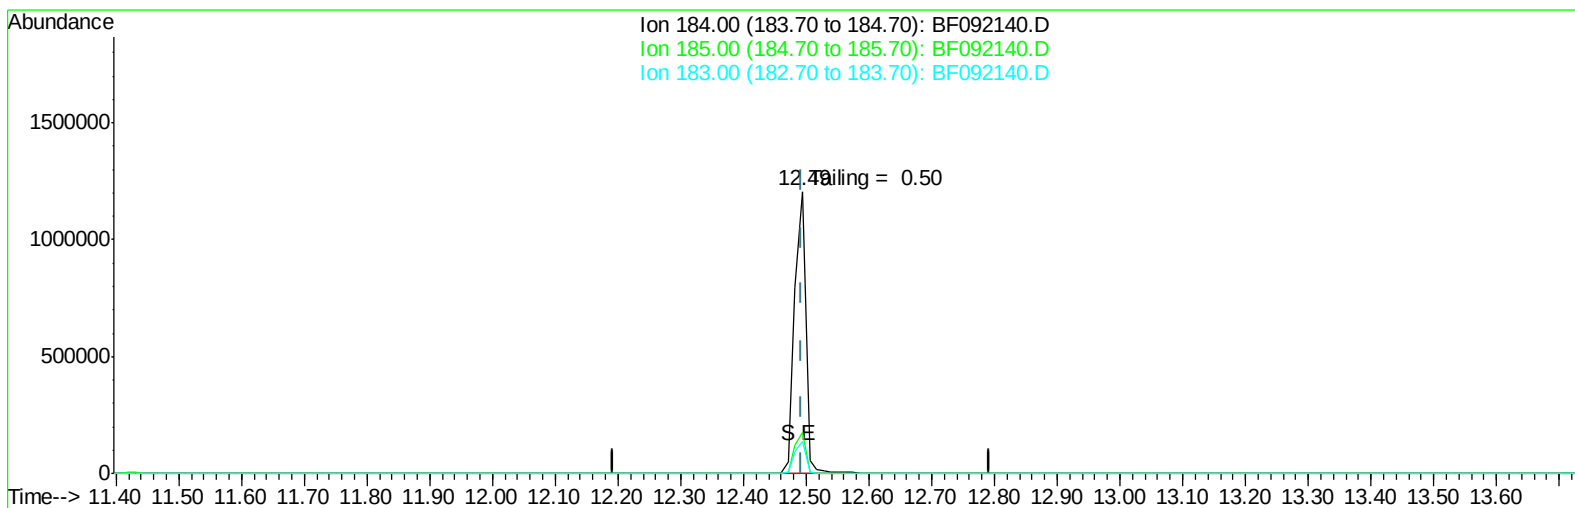

TIC: BF092140.D

(76) Benzidine

12.494min (+0.000) 0.00ng

response 1489553

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.42
183.00	11.50	11.52
0.00	0.00	0.00