


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF010917\
 Data File : BF092166.D
 Acq On : 10 Jan 2017 4:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

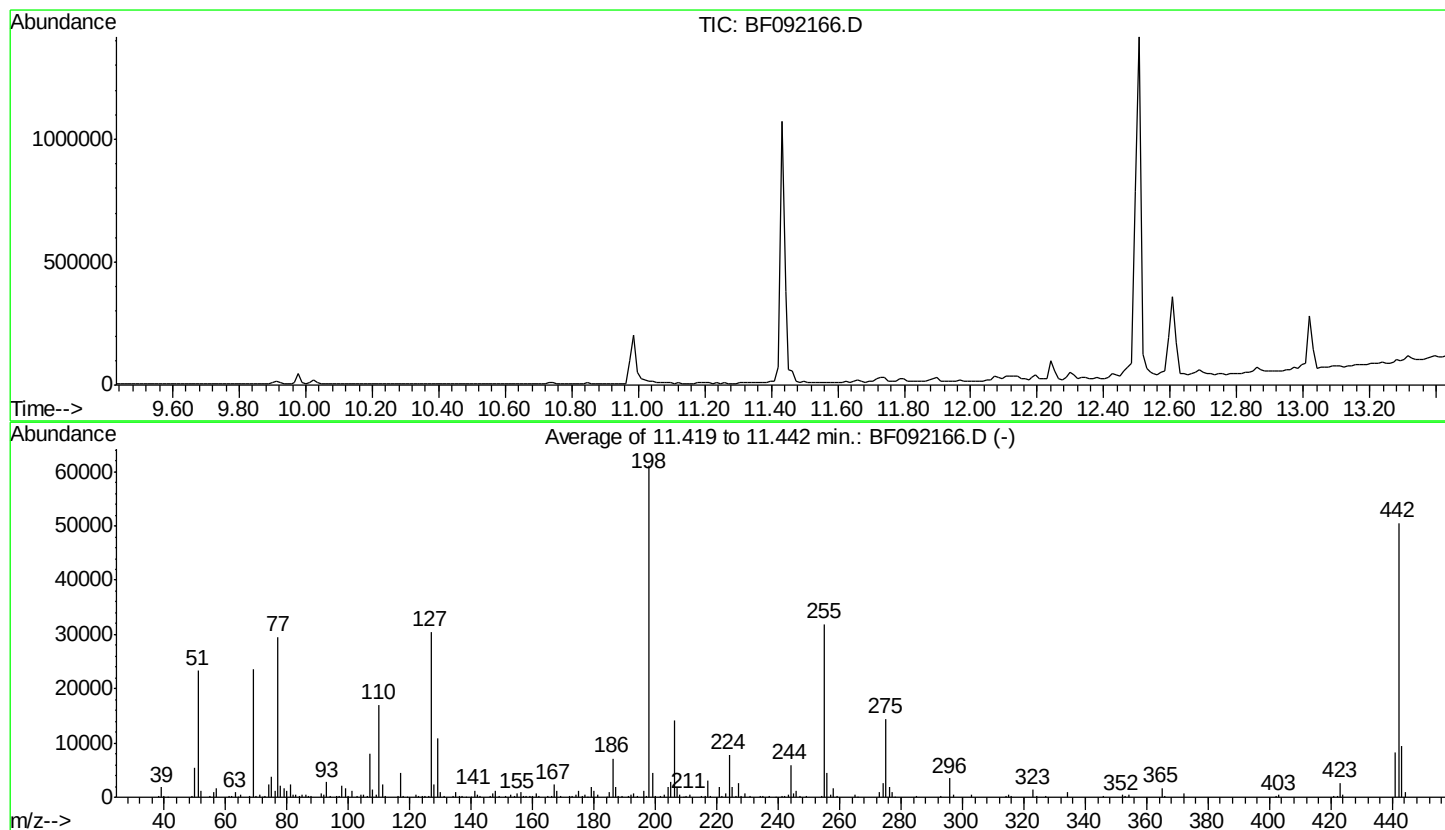

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	23294	PASS
68	69	0.00	2	1.3	295	PASS
69	198	0.00	100	38.4	23495	PASS
70	69	0.00	2	0.6	136	PASS
127	198	10	80	49.9	30492	PASS
197	198	0.00	2	0.4	268	PASS
198	198	100	100	100.0	61113	PASS
199	198	5	9	7.2	4417	PASS
275	198	10	60	23.7	14470	PASS
365	198	1	100	2.8	1723	PASS
441	442	0.01	24	16.2	8216	PASS
442	198	50	100	82.8	50586	PASS
443	442	15	24	18.8	9500	PASS