
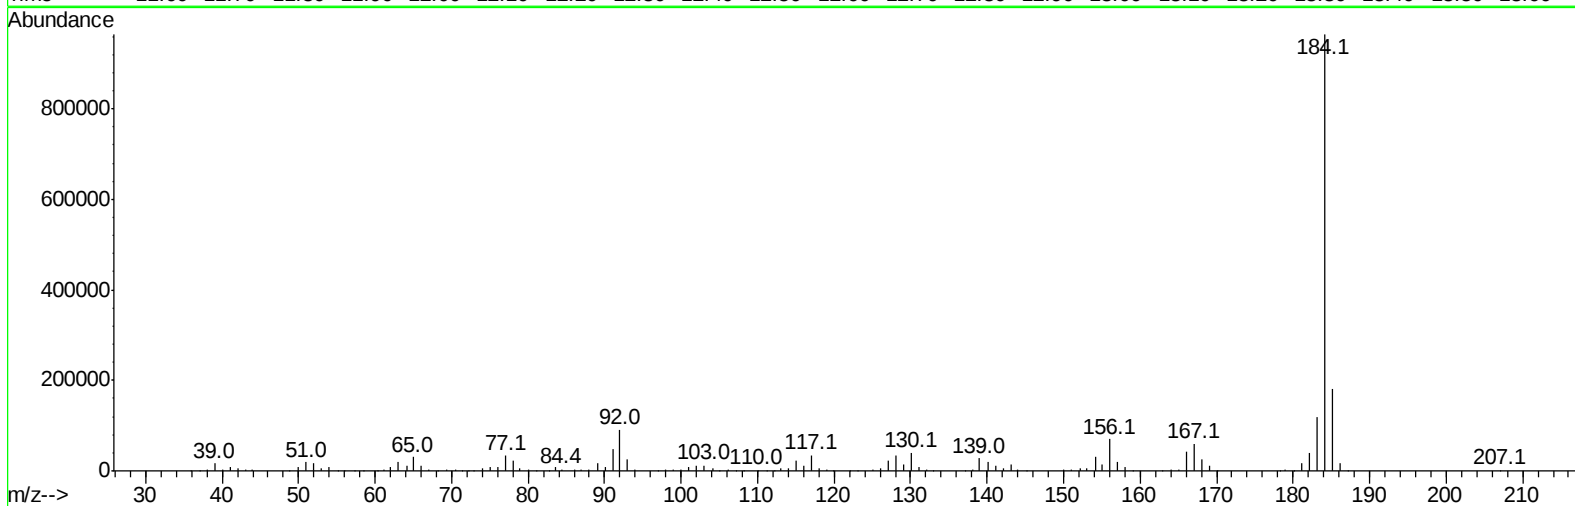


Data Path : Z:\HPCHEM1\BNA F\DATA\BF010918\
Data File : BF101952.D
Acq On : 9 Jan 2018 15:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 05:20:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 15:20:36 2018
Response via : Initial Calibration

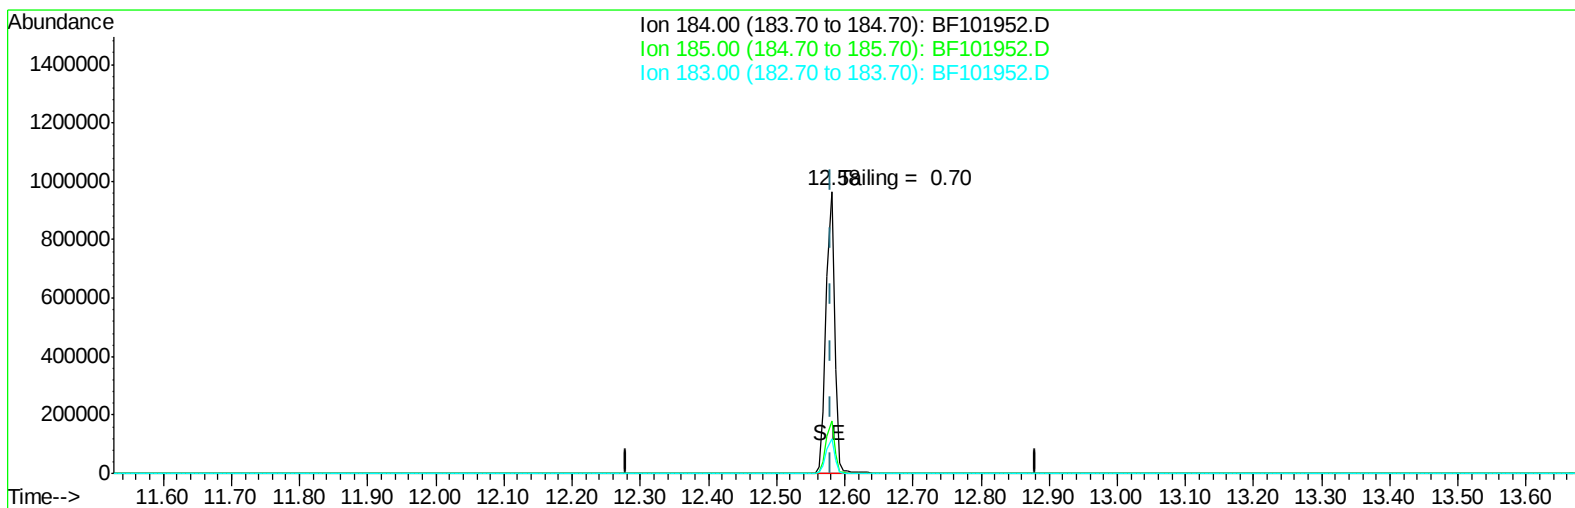

TIC: BF101952.D

(76) Benzidine



12.580min (+0.000) 0.00ng

response 815228

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	18.76
183.00	11.60	12.28
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF010918\
Data File : BF101952.D
Acq On : 9 Jan 2018 15:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 05:20:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 15:20:36 2018
Response via : Initial Calibration

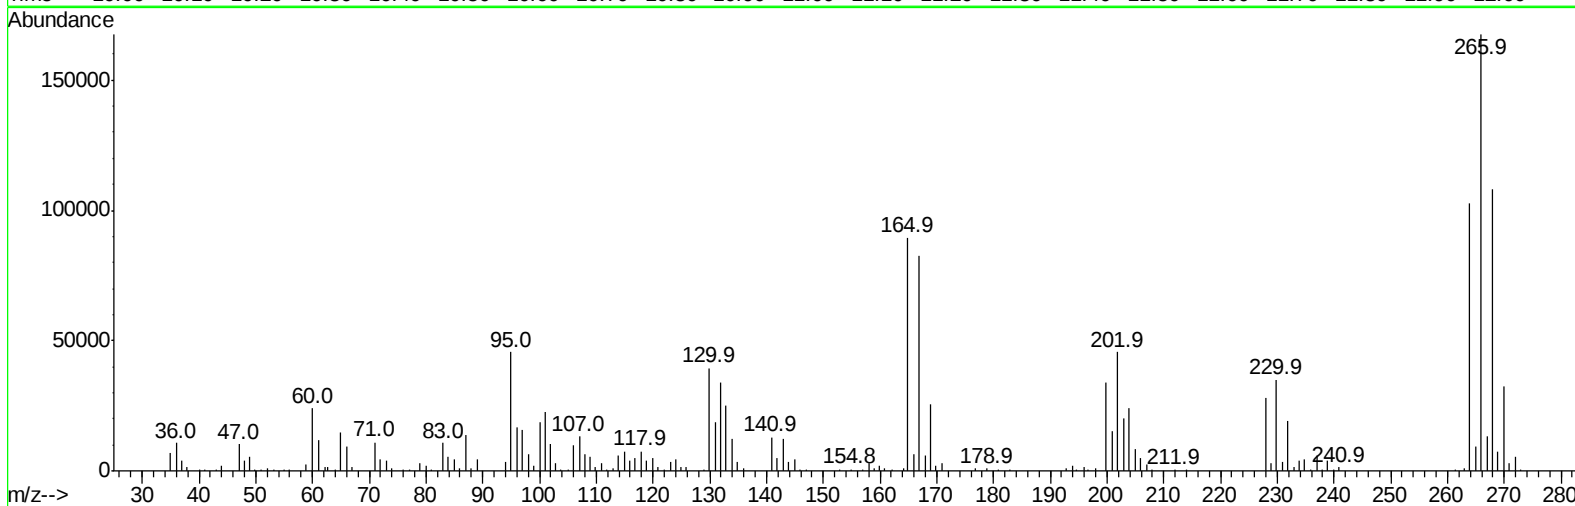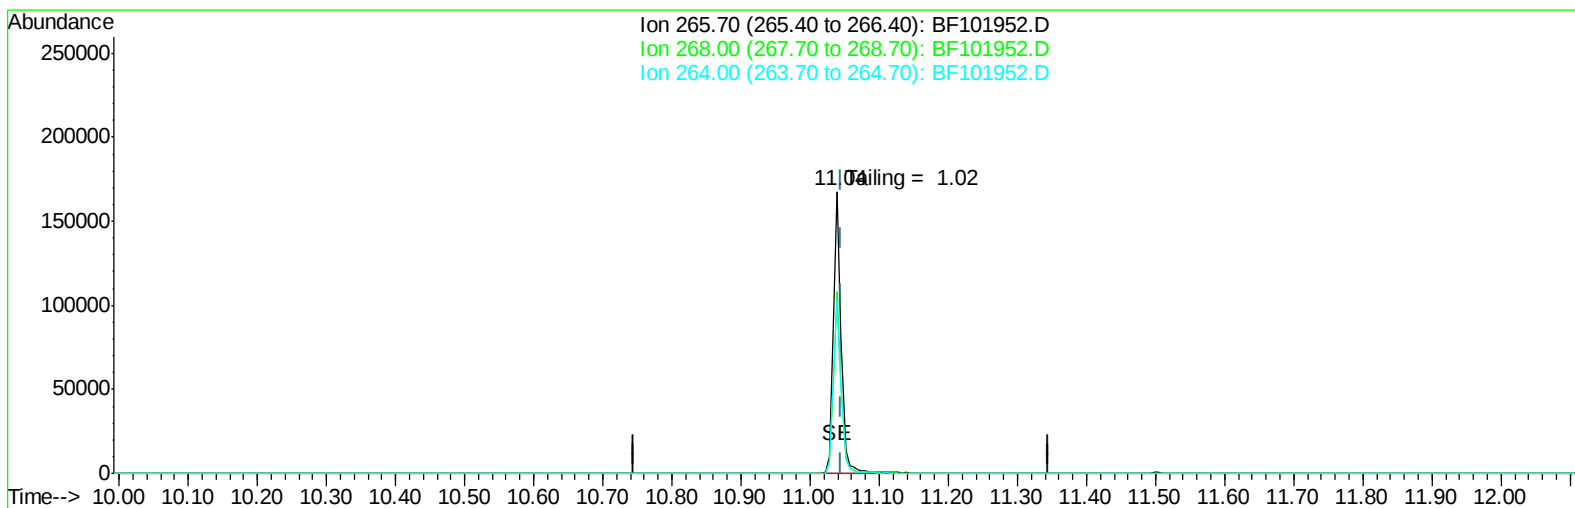

TIC: BF101952.D

(69) Pentachlorophenol (C)



11.039min (-0.006) 34498.29ng

response 132177

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.39
264.00	61.90	61.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF010918\
Data File : BF101952.D
Acq On : 9 Jan 2018 15:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 05:20:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 15:20:36 2018
Response via : Initial Calibration

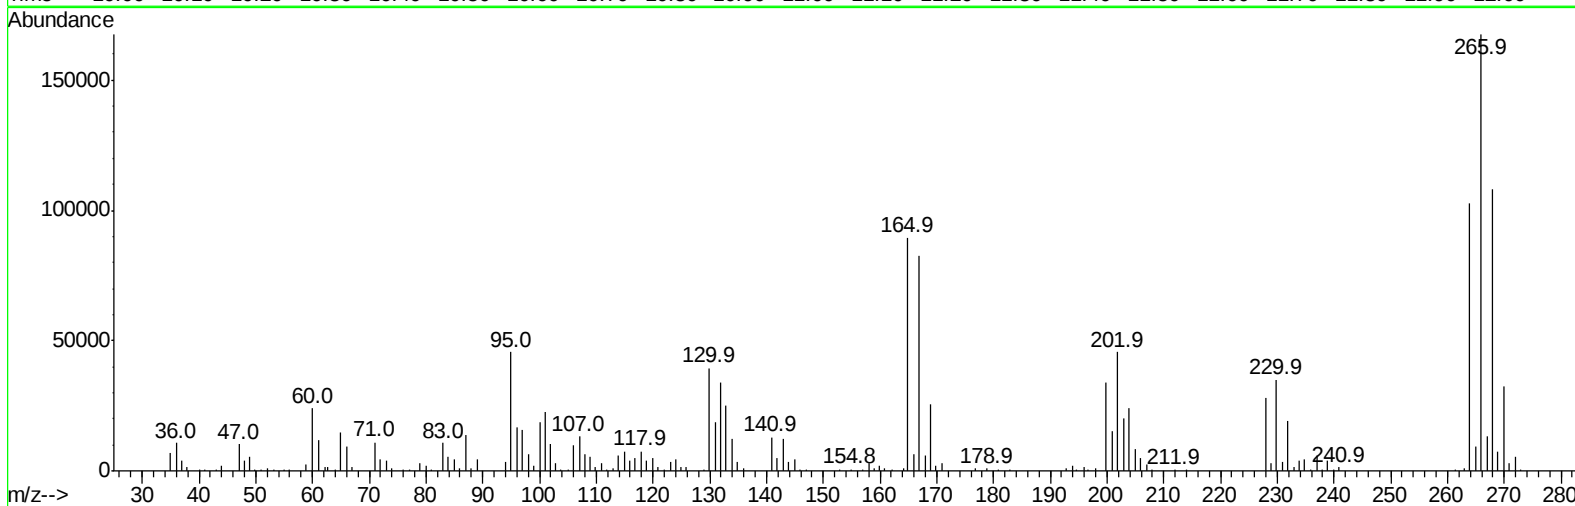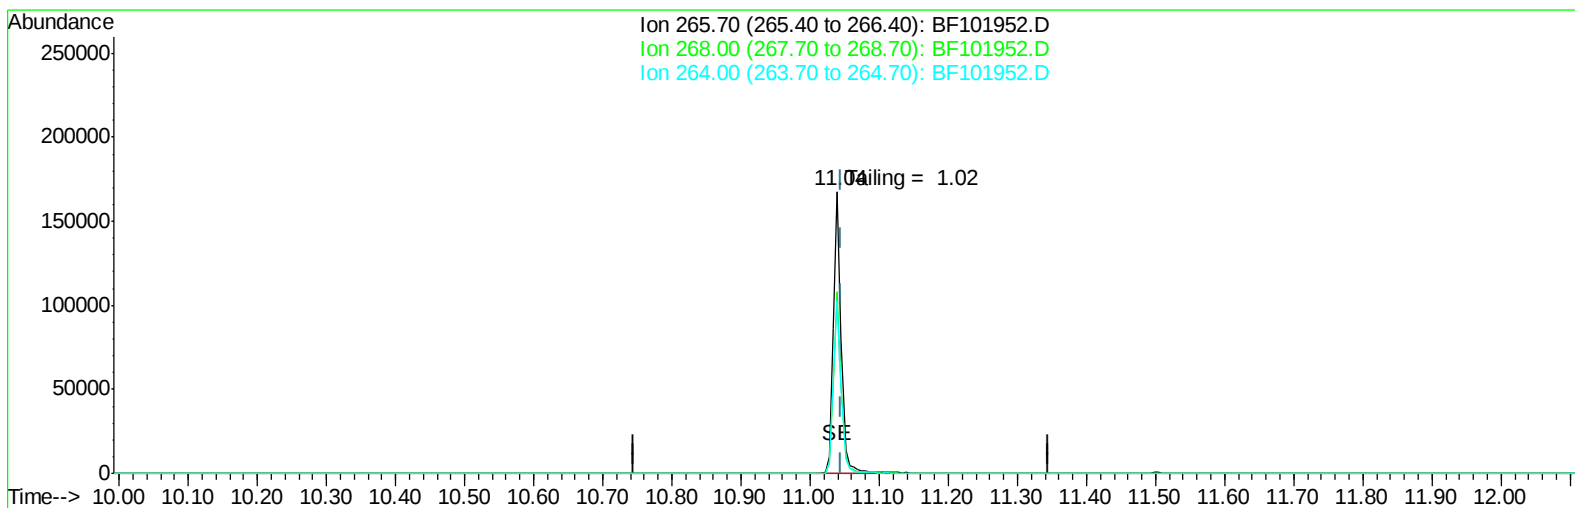

TIC: BF101952.D

(69) Pentachlorophenol (C)

11.039min (-0.006) 34498.29ng

response 132177

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.39
264.00	61.90	61.40
0.00	0.00	0.00