


Data Path : Z:\HPCHEM1\BNA F\Data\BF010918\
 Data File : BF101943.D
 Acq On : 9 Jan 2018 10:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 09 15:20:36 2018

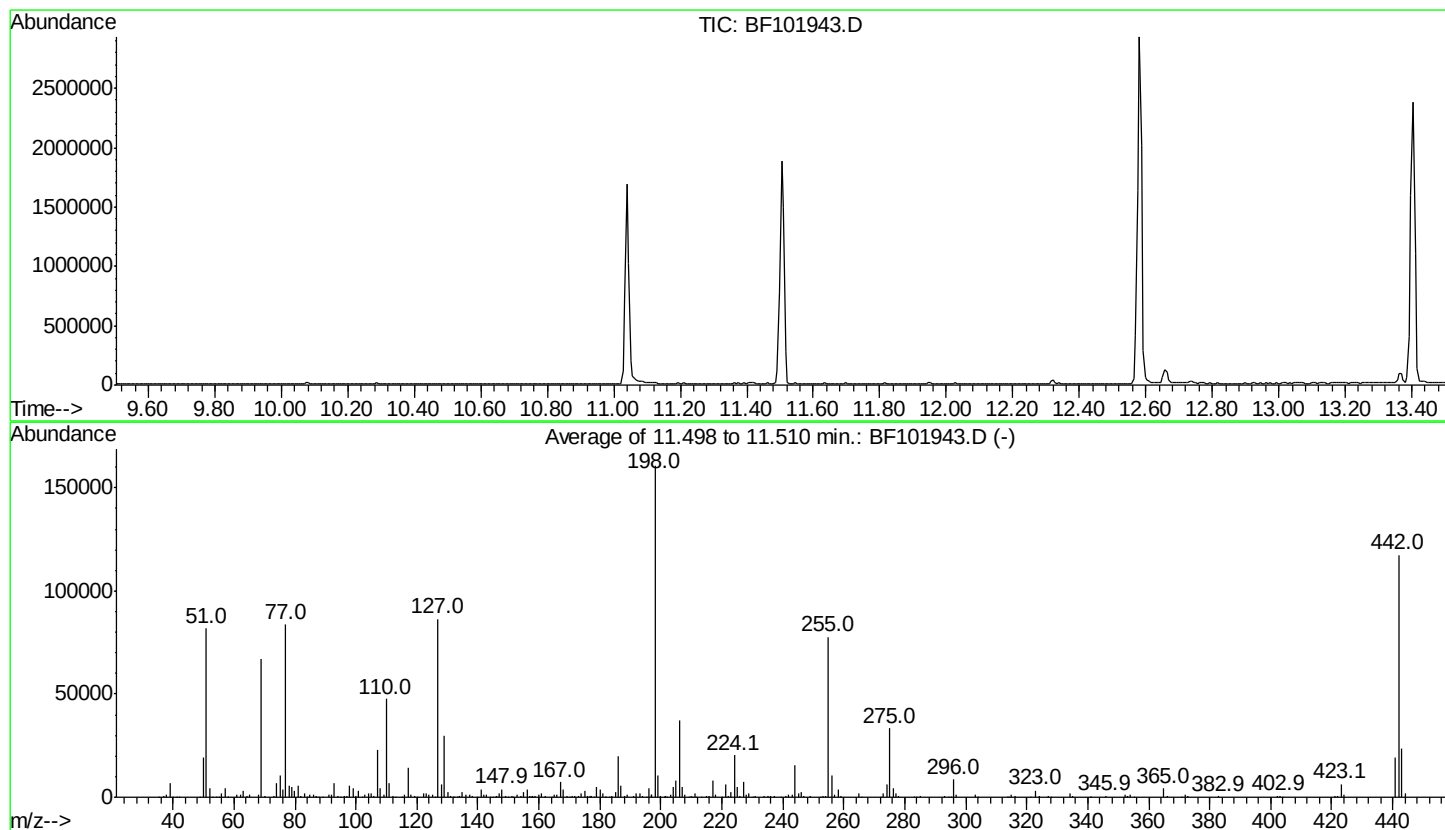

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	81717	PASS
68	69	0.00	2	1.8	1178	PASS
69	198	0.00	100	41.8	67195	PASS
70	69	0.00	2	0.9	604	PASS
127	198	10	80	53.7	86336	PASS
197	198	0.00	2	0.8	1246	PASS
198	198	100	100	100.0	160762	PASS
199	198	5	9	6.6	10599	PASS
275	198	10	60	20.8	33460	PASS
365	198	1	100	2.6	4179	PASS
441	443	0.01	100	81.7	19244	PASS
442	198	50	100	73.0	117378	PASS
443	442	15	24	20.1	23542	PASS