


Data Path : Z:\HPCHEM1\BNA F\Data\BF010918\
Data File : BF101952.D
Acq On : 9 Jan 2018 15:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 15:20:36 2018

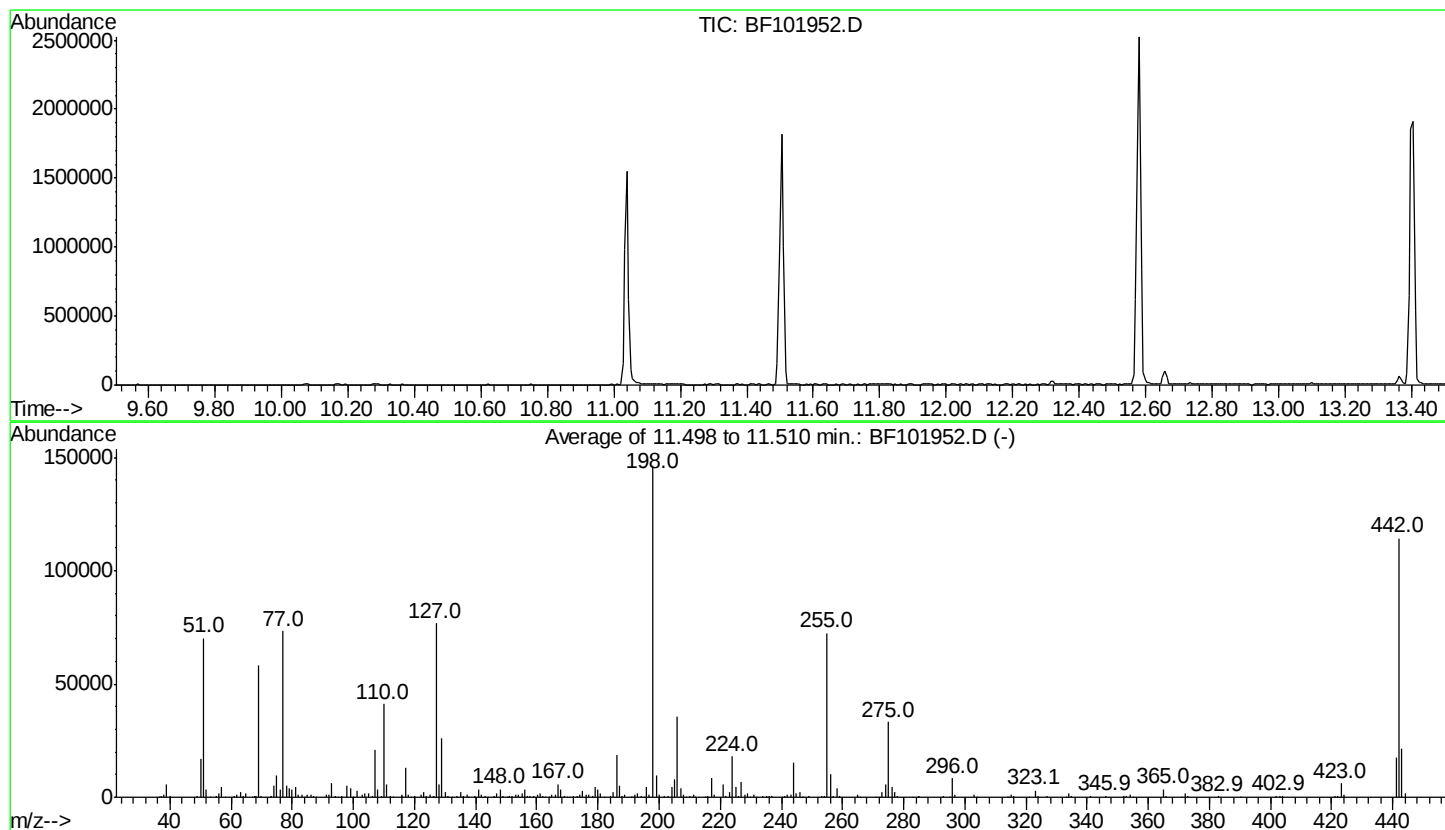

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	70056	PASS
68	69	0.00	2	0.9	508	PASS
69	198	0.00	100	39.9	58365	PASS
70	69	0.00	2	0.6	365	PASS
127	198	10	80	52.3	76597	PASS
197	198	0.00	2	0.7	1031	PASS
198	198	100	100	100.0	146349	PASS
199	198	5	9	6.6	9653	PASS
275	198	10	60	22.7	33194	PASS
365	198	1	100	2.3	3432	PASS
441	443	0.01	100	82.2	17738	PASS
442	198	50	100	78.2	114397	PASS
443	442	15	24	18.9	21570	PASS