
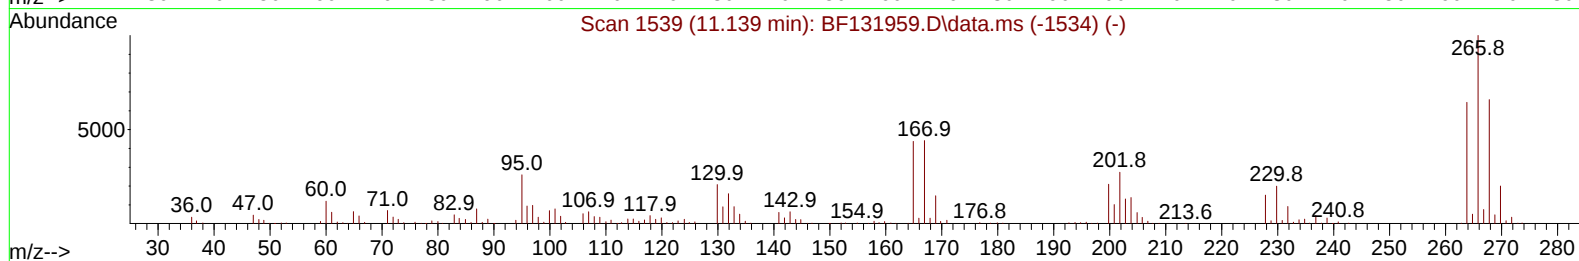
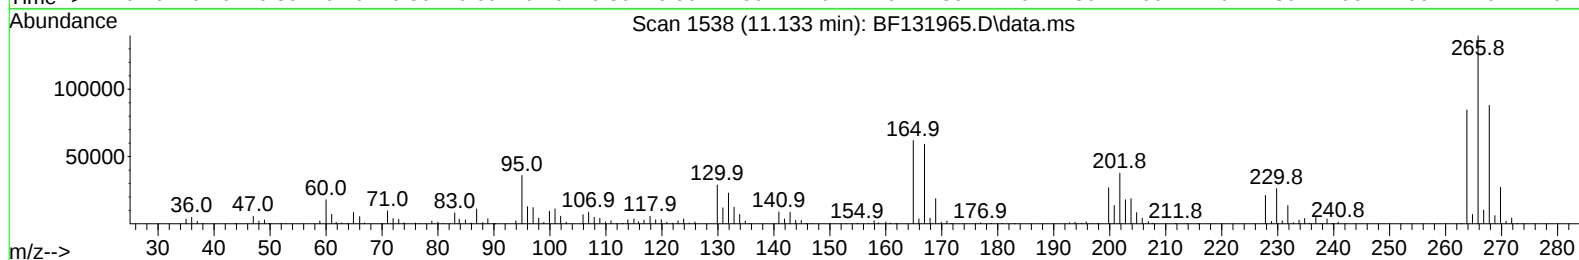


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010923\
Data File : BF131965.D
Acq On : 09 Jan 2023 16:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 04:54:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 00:32:25 2023
Response via : Initial Calibration

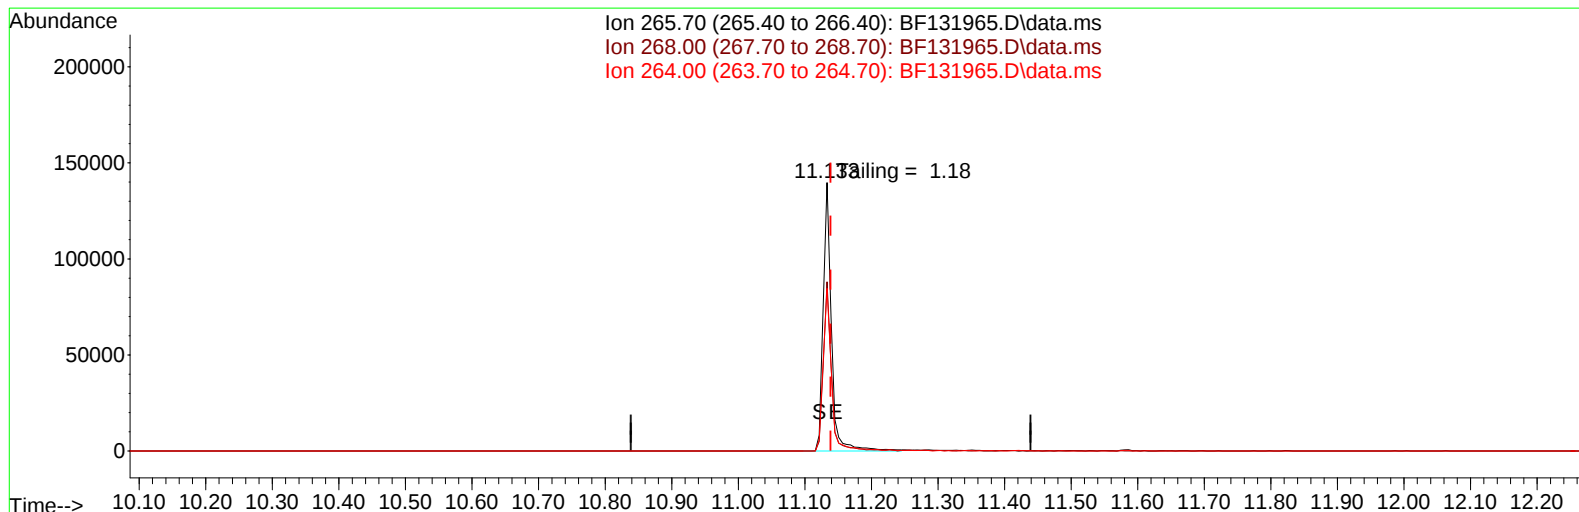

TIC: BF131965.D\data.ms

(70) Pentachlorophenol (C)




11.133min (-0.006) 18570.05 ng m

response 119919

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	63.04
264.00	64.50	60.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010923\
Data File : BF131965.D
Acq On : 09 Jan 2023 16:10
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 04:54:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 00:32:25 2023
Response via : Initial Calibration

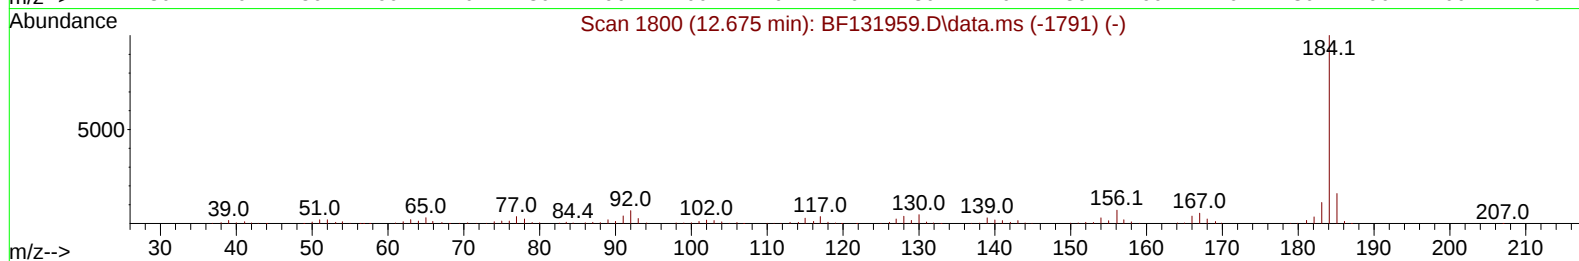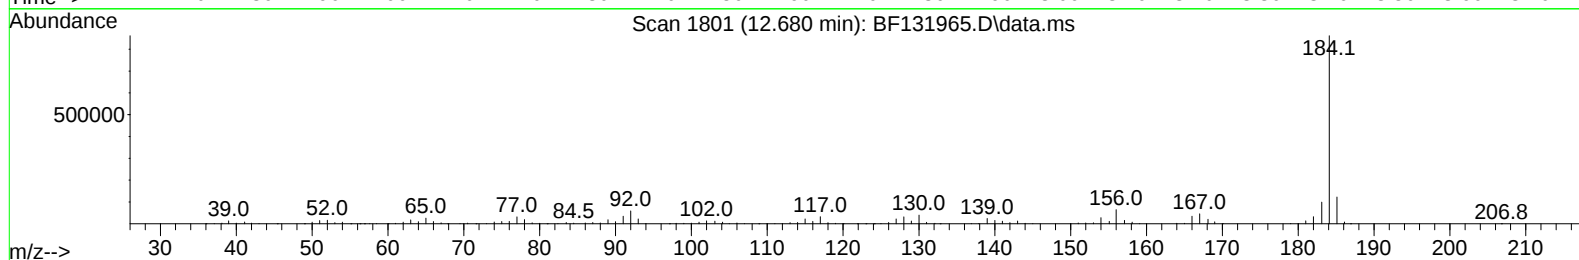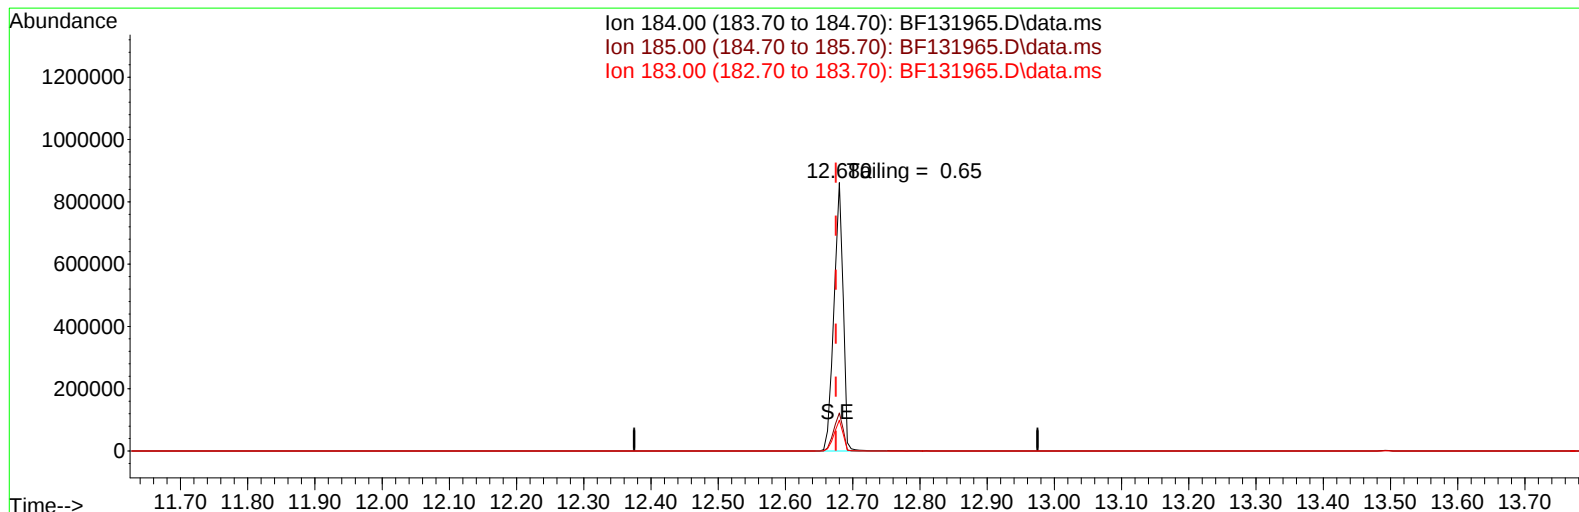

TIC: BF131965.D\data.ms

(77) Benzidine

12.680min (+ 0.005) 0.00 ng

response 817476

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.21
183.00	11.20	11.50
0.00	0.00	0.00