


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010923\
Data File : BF131954.D
Acq On : 09 Jan 2023 10:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 10 00:32:25 2023

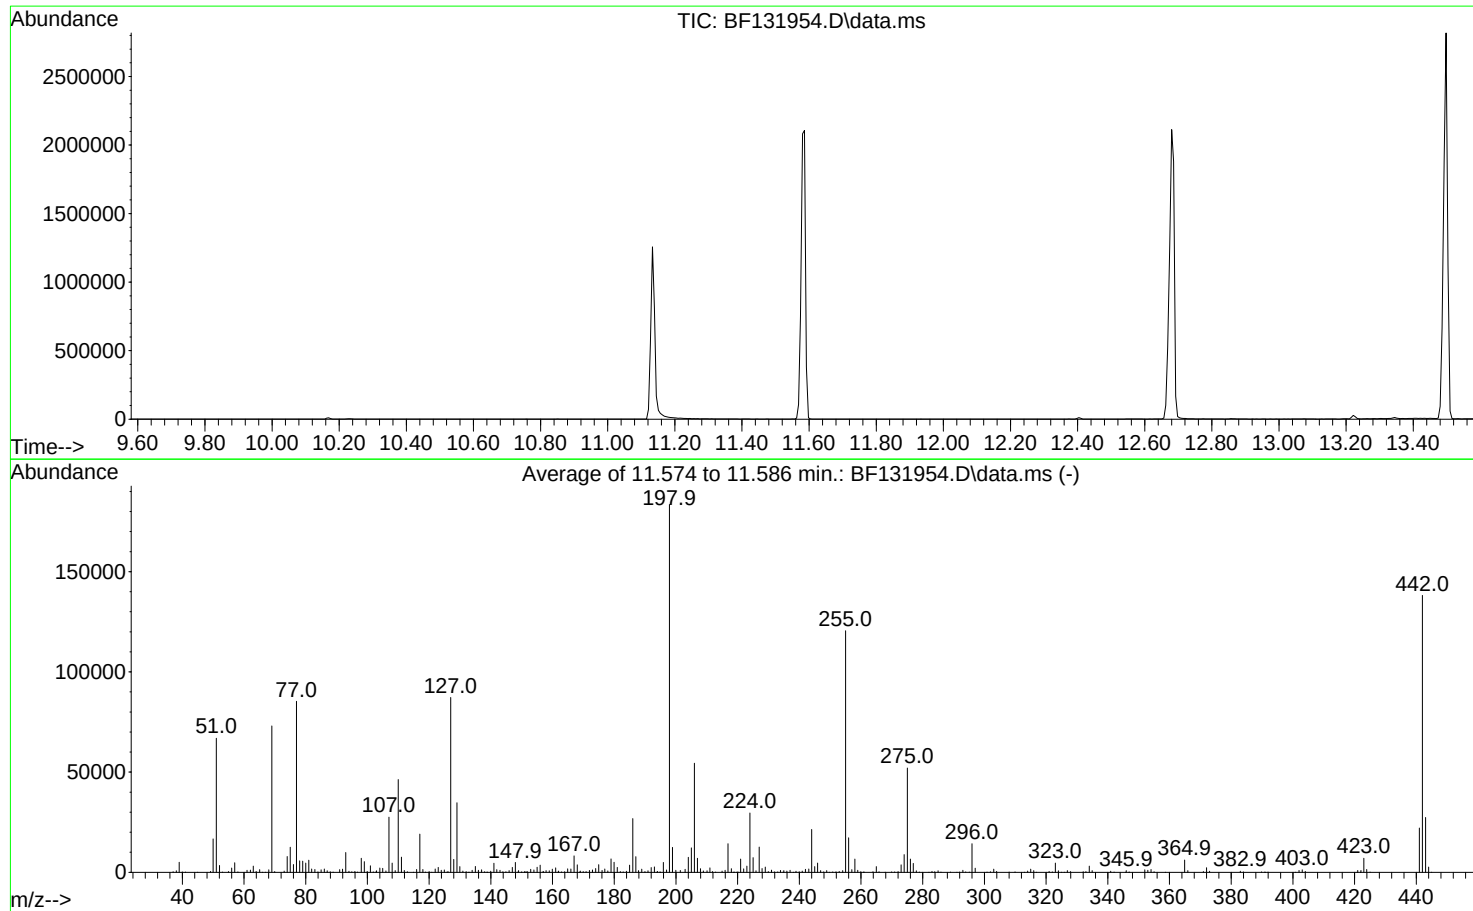




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	66843	PASS
68	69	0.00	2	1.8	1287	PASS
69	198	0.00	100	39.8	73021	PASS
70	69	0.00	2	0.5	384	PASS
127	198	10	80	47.5	87272	PASS
197	198	0.00	2	0.6	1130	PASS
198	198	100	100	100.0	183573	PASS
199	198	5	9	6.8	12435	PASS
275	198	10	60	28.3	52011	PASS
365	198	1	100	3.3	6149	PASS
441	198	0.01	100	12.0	22098	PASS
442	442	50	100	100.0	138144	PASS
443	442	15	24	19.8	27391	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010923\
Data File : BF131954.D
Acq On : 09 Jan 2023 10:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 10 05:38:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 00:32:25 2023
Response via : Initial Calibration

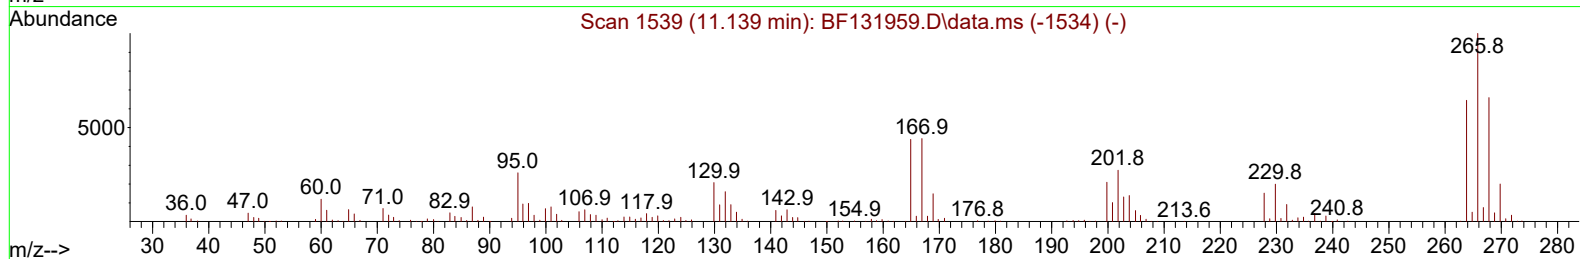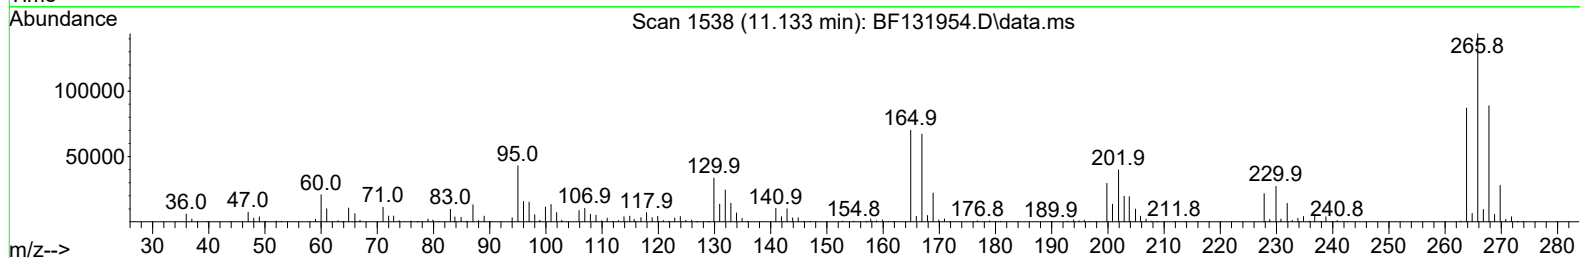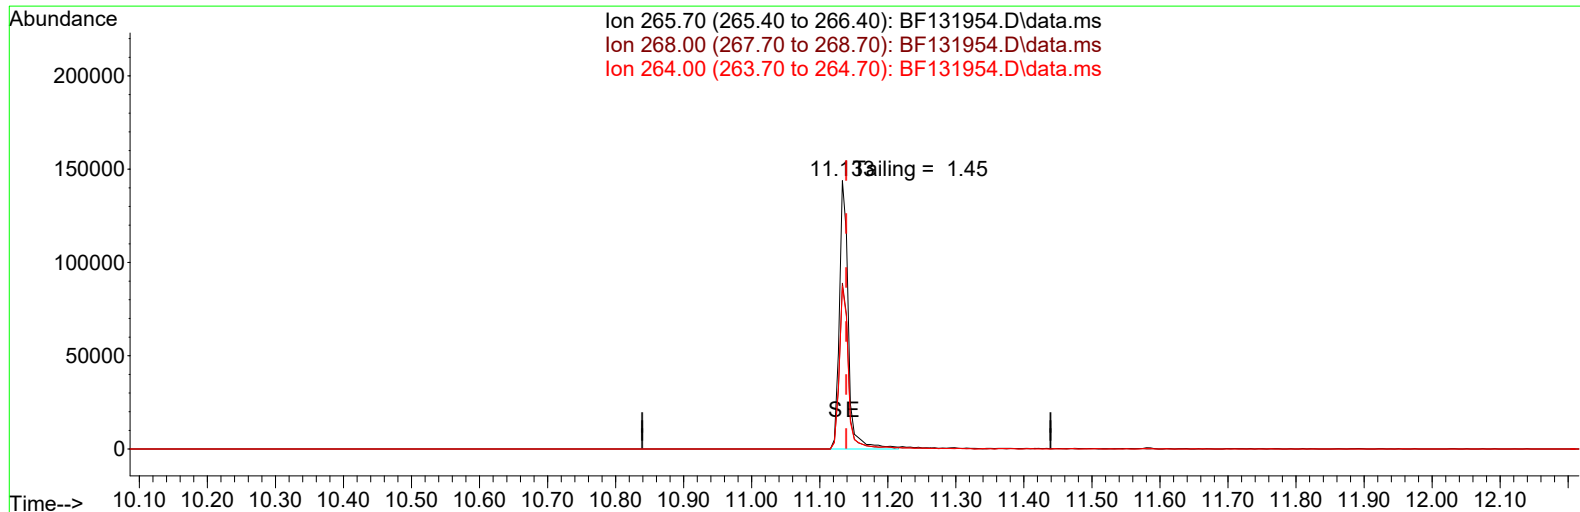

TIC: BF131954.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.006) 19818.25 ng




response 131941

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	61.77
264.00	64.50	60.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010923\
Data File : BF131954.D
Acq On : 09 Jan 2023 10:16
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 10 05:38:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 00:32:25 2023
Response via : Initial Calibration

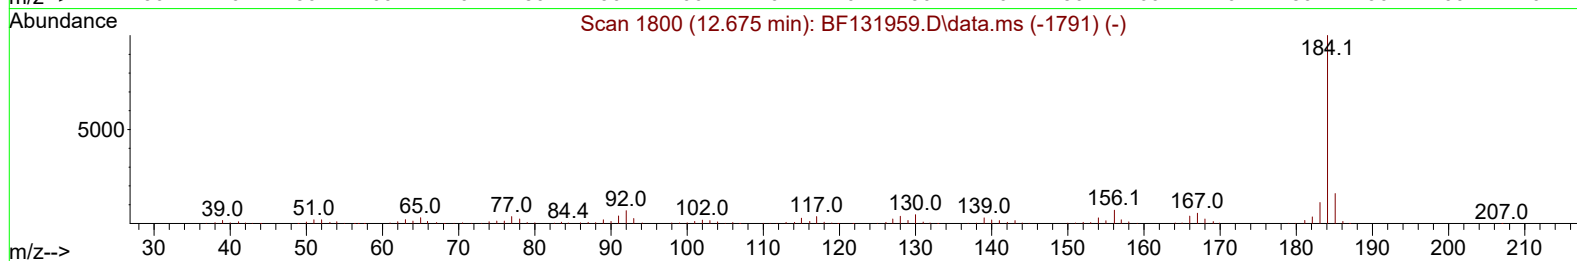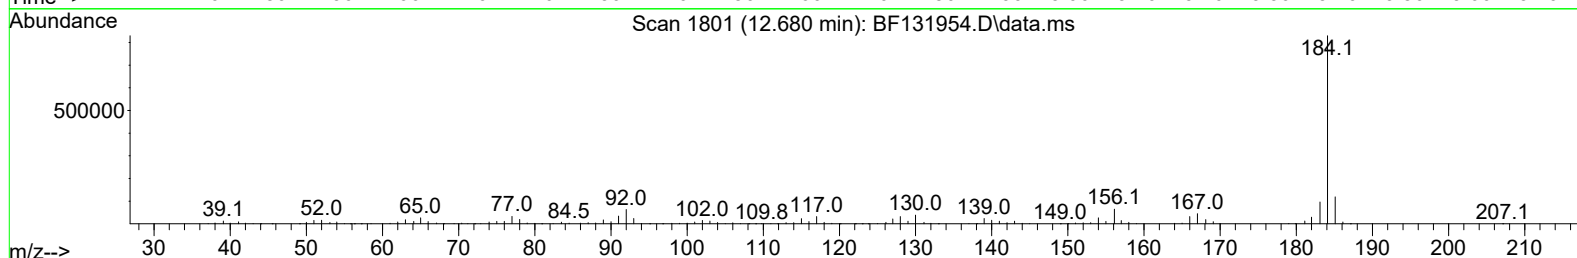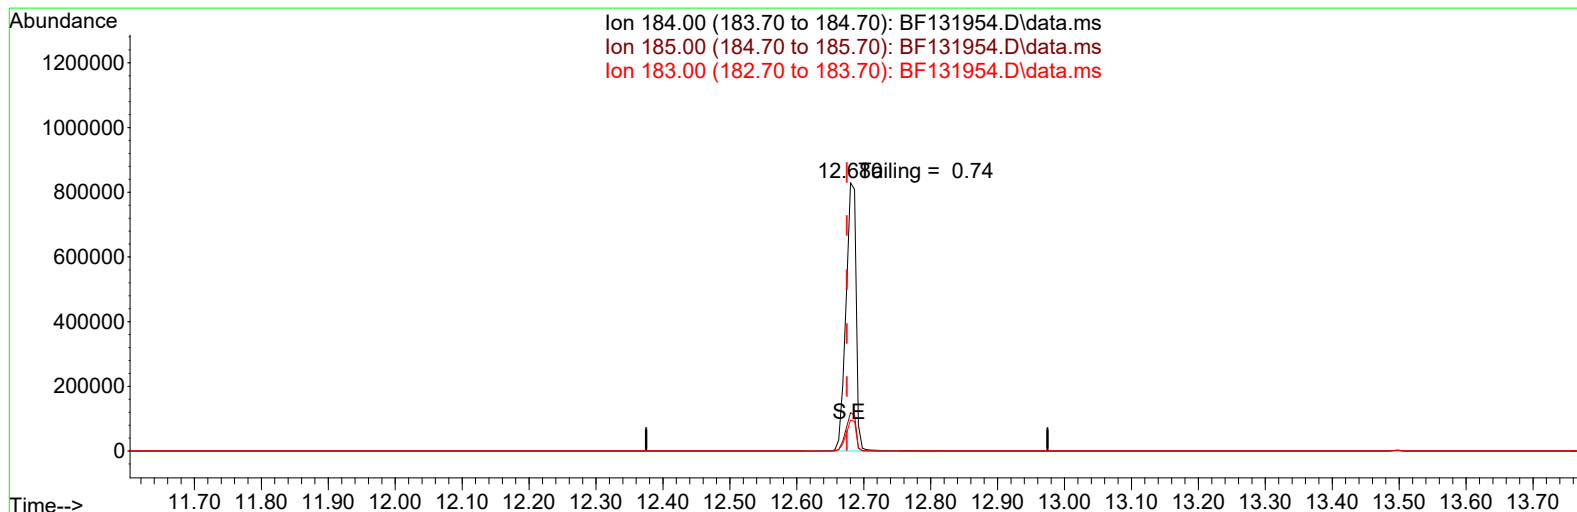

TIC: BF131954.D\data.ms

(77) Benzidine

12.680min (+ 0.005) 0.00 ng

response 876837

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.32
183.00	11.20	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/9/2023	BNA_F	<u>BF131954.D</u>
Compound Name	Response	Retention Time
DDT	465212	13.498
DDD	4681	13.221
DDE	731	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5412	470624	1.15

Instrument :
BNA_F
ClientSampleId :
DFTPP