


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF010923\  
Data File : BF131965.D  
Acq On : 09 Jan 2023 16:10  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF010923.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Jan 10 00:32:25 2023

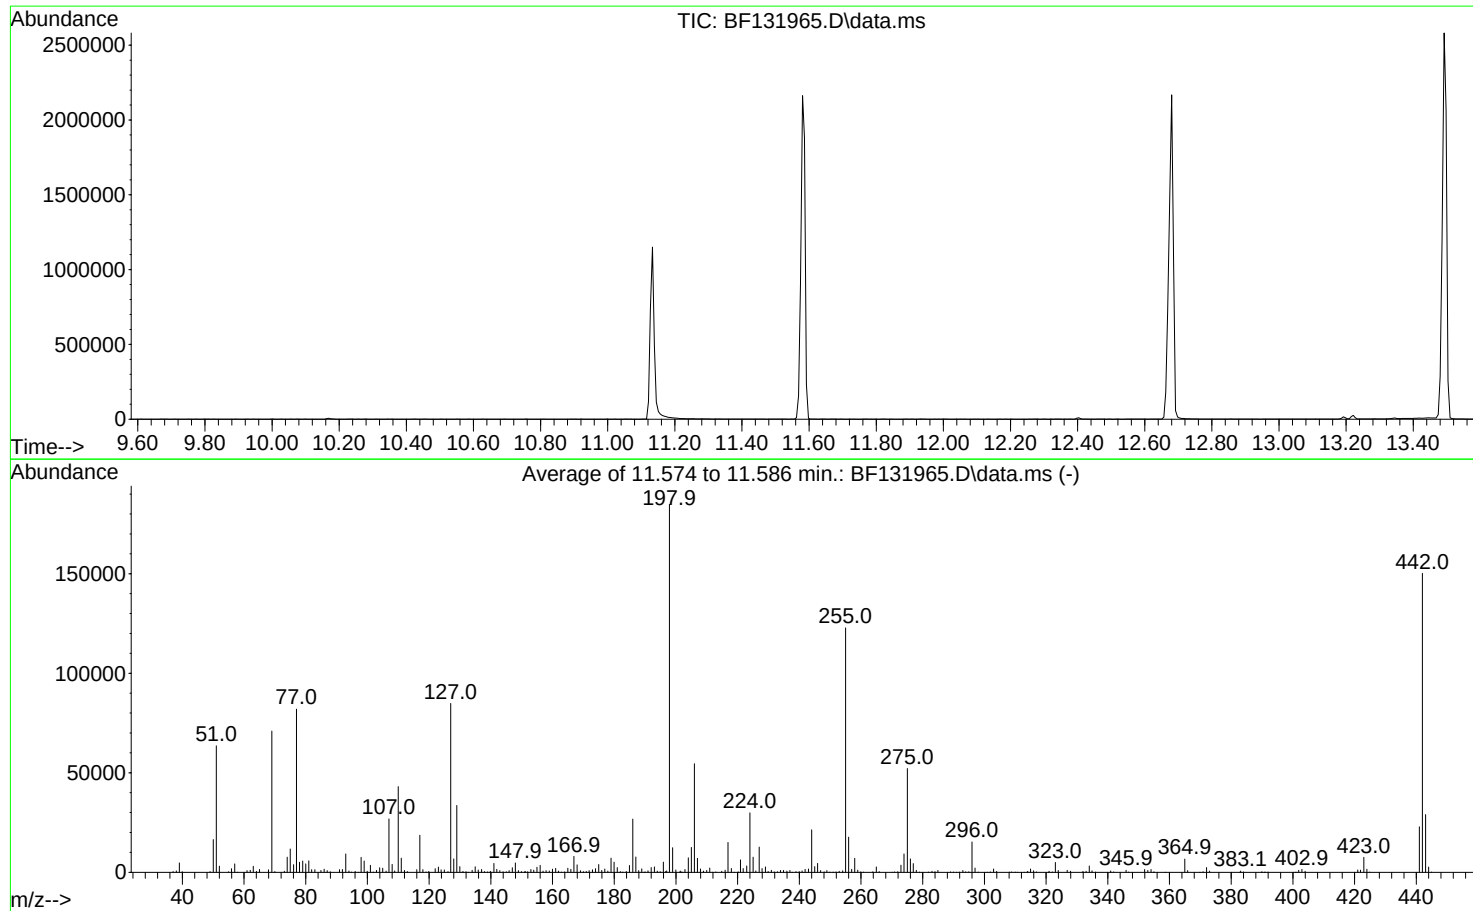




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.4         | 63573      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1251       | PASS                |
| 69             | 198             | 0.00            | 100             | 38.4         | 70976      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 381        | PASS                |
| 127            | 198             | 10              | 80              | 45.9         | 84861      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 664        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 184824     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 12351      | PASS                |
| 275            | 198             | 10              | 60              | 28.2         | 52136      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 6617       | PASS                |
| 441            | 198             | 0.01            | 100             | 12.4         | 22894      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 150245     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 28998      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF010923\  
Data File : BF131965.D  
Acq On : 09 Jan 2023 16:10  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jan 10 04:54:15 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF010923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 10 00:32:25 2023  
Response via : Initial Calibration

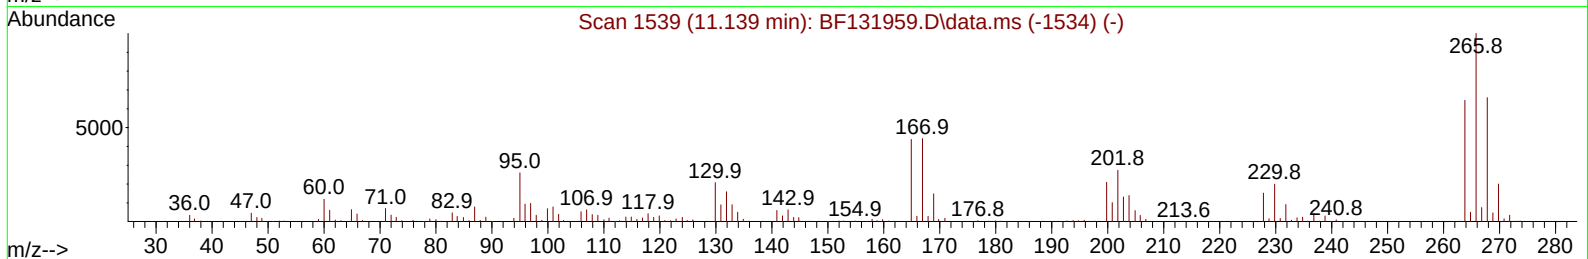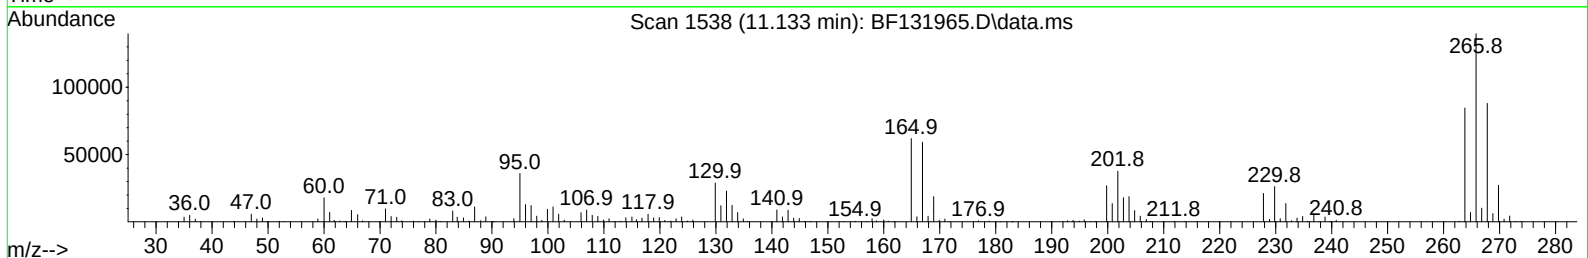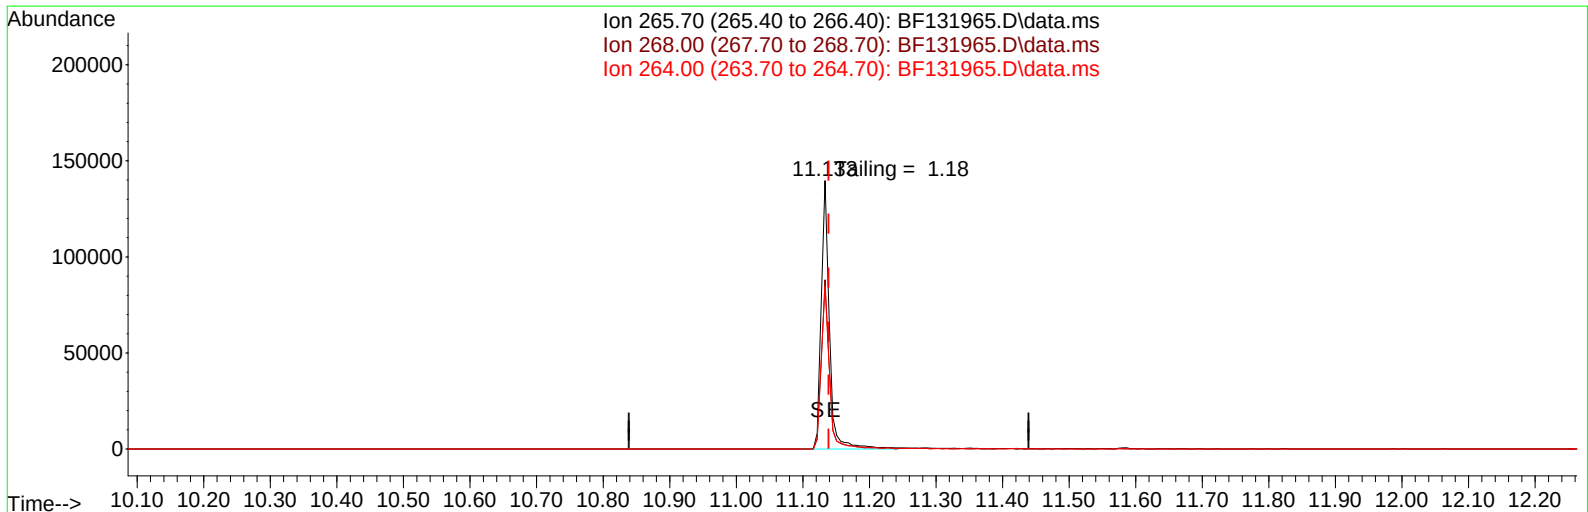

TIC: BF131965.D\data.ms

**(70) Pentachlorophenol (C)**

11.133min (-0.006) 18570.05 ng m




response 119919

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.90  | 63.04  |
| 264.00 | 64.50  | 60.56  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF010923\  
Data File : BF131965.D  
Acq On : 09 Jan 2023 16:10  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Jan 10 04:54:15 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF010923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jan 10 00:32:25 2023  
Response via : Initial Calibration

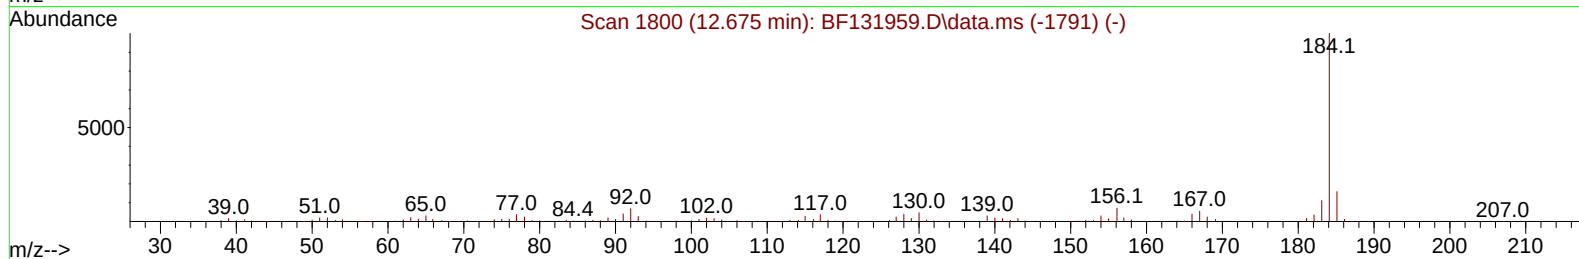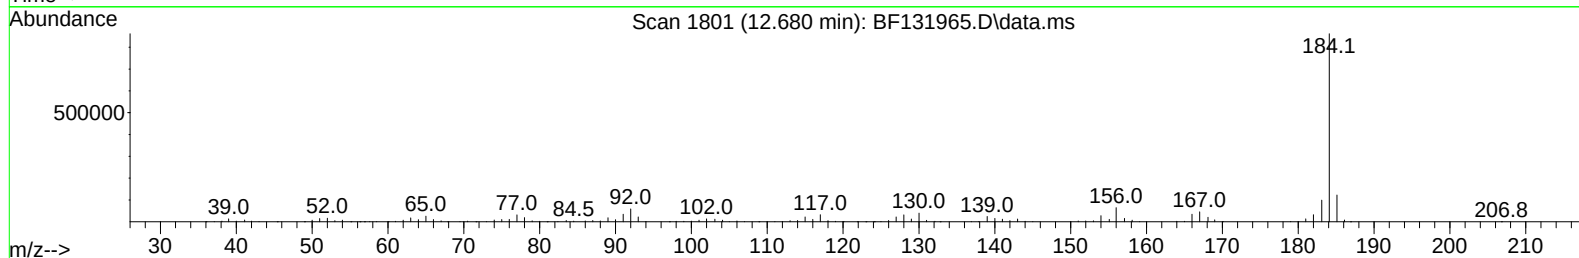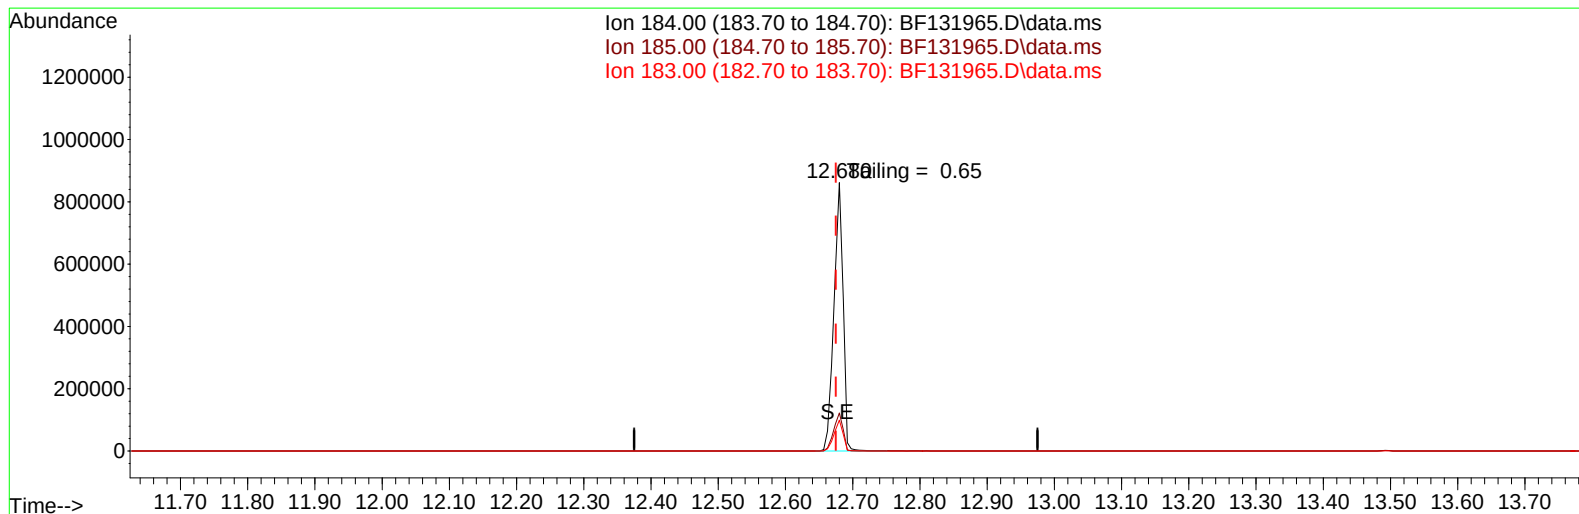

TIC: BF131965.D\data.ms

(77) Benzidine

12.680min (+ 0.005) 0.00 ng

response 817476

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 16.00  | 14.21  |
| 183.00 | 11.20  | 11.50  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/9/2023      | BNA_F            | <u>BF131965.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 445700           | 13.492             |
| DDD           | 7132             | 13.221             |
| DDE           | 400              | 12.857             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7532          | 453232           | 1.66               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP