
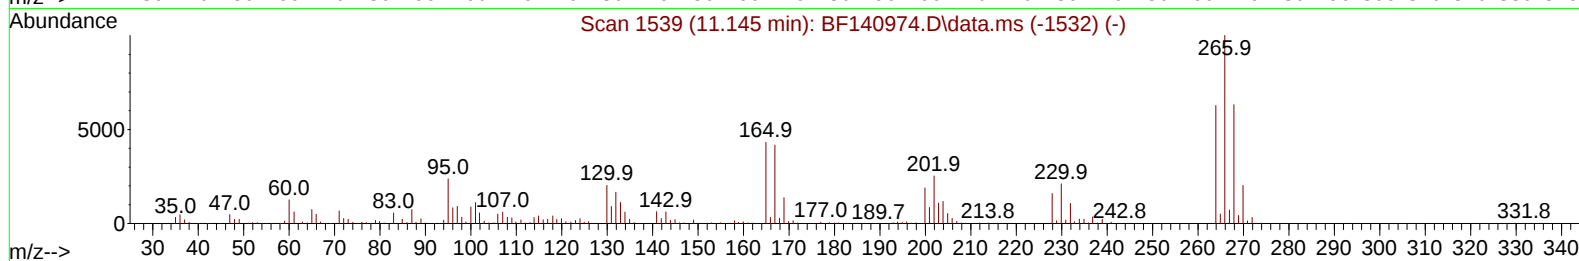
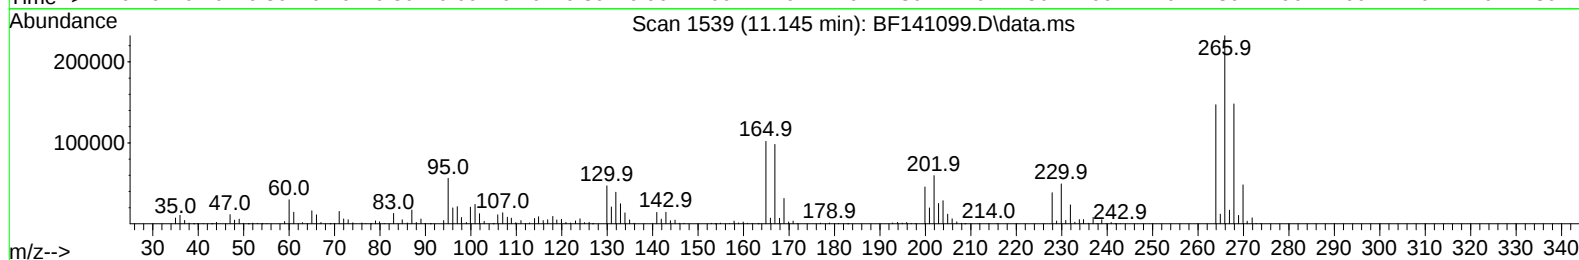


Quant Time: Jan 09 12:03:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

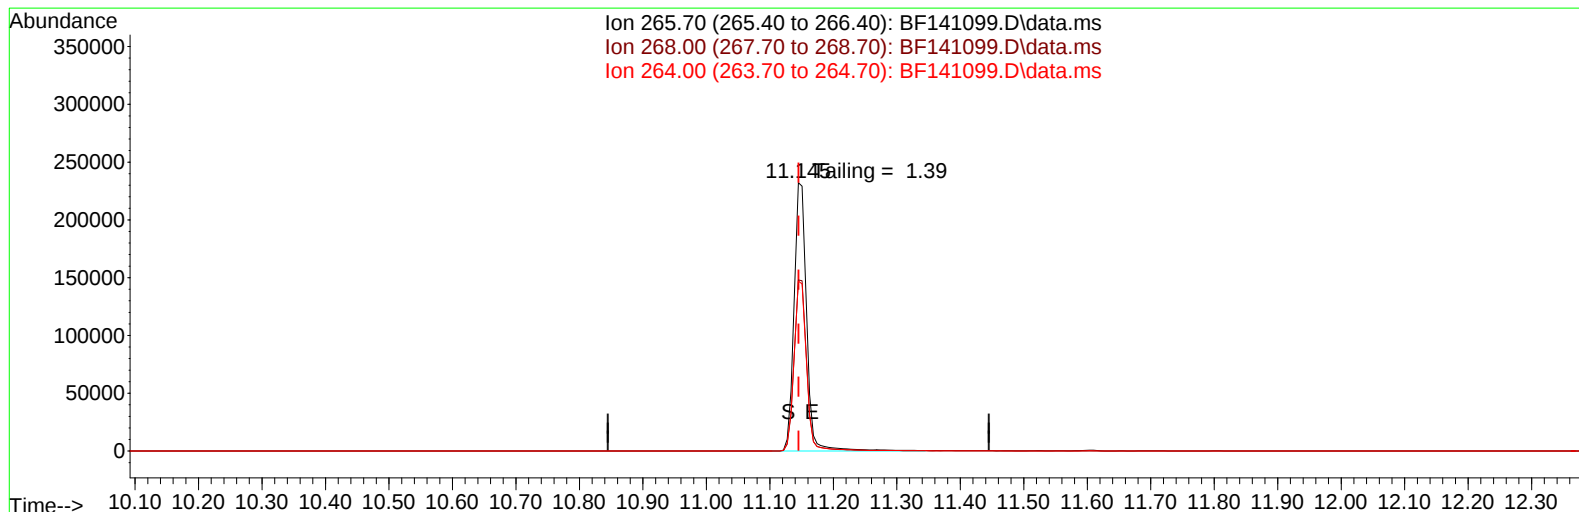

TIC: BF141099.D\data.ms

(70) Pentachlorophenol (C)




11.145min (0.000) 27821.83 ng

response 323344

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.74
264.00	62.80	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010925\
Data File : BF141099.D
Acq On : 09 Jan 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 09 12:03:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

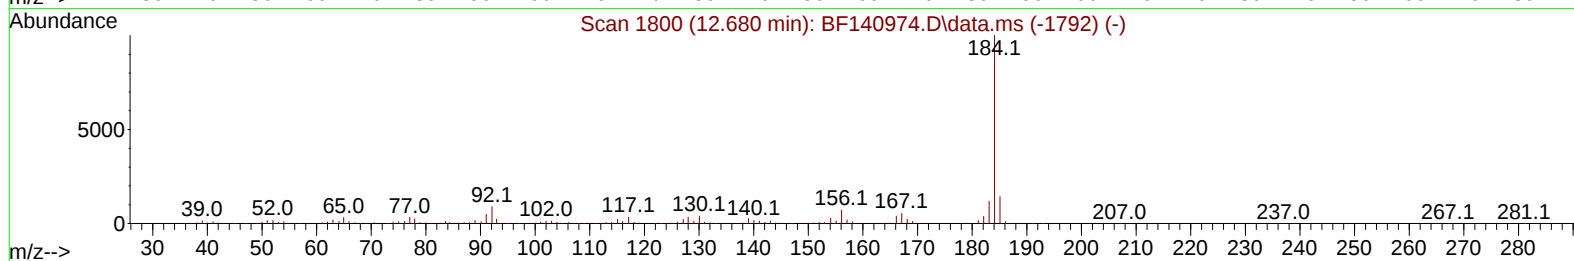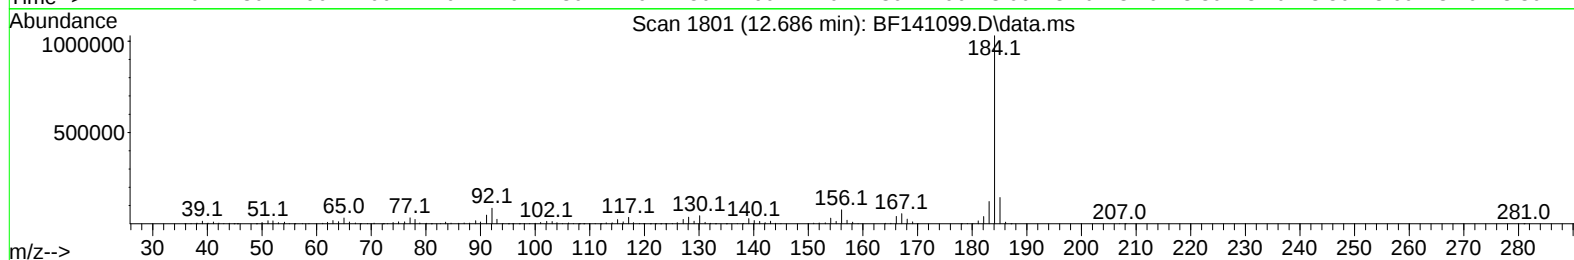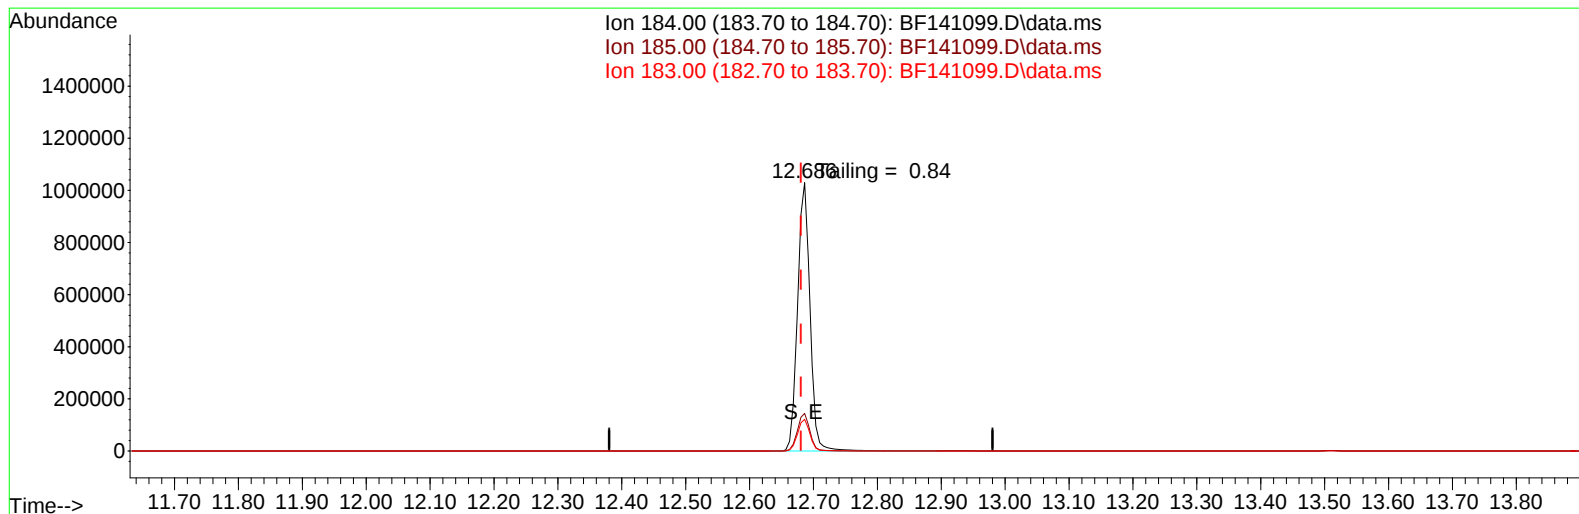

TIC: BF141099.D\data.ms

(77) Benzidine**12.686min (+ 0.006) 59252.02 ng****response 1399996**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.00
183.00	11.70	11.85
0.00	0.00	0.00