


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010925\
Data File : BF141099.D
Acq On : 09 Jan 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 27 00:31:16 2024

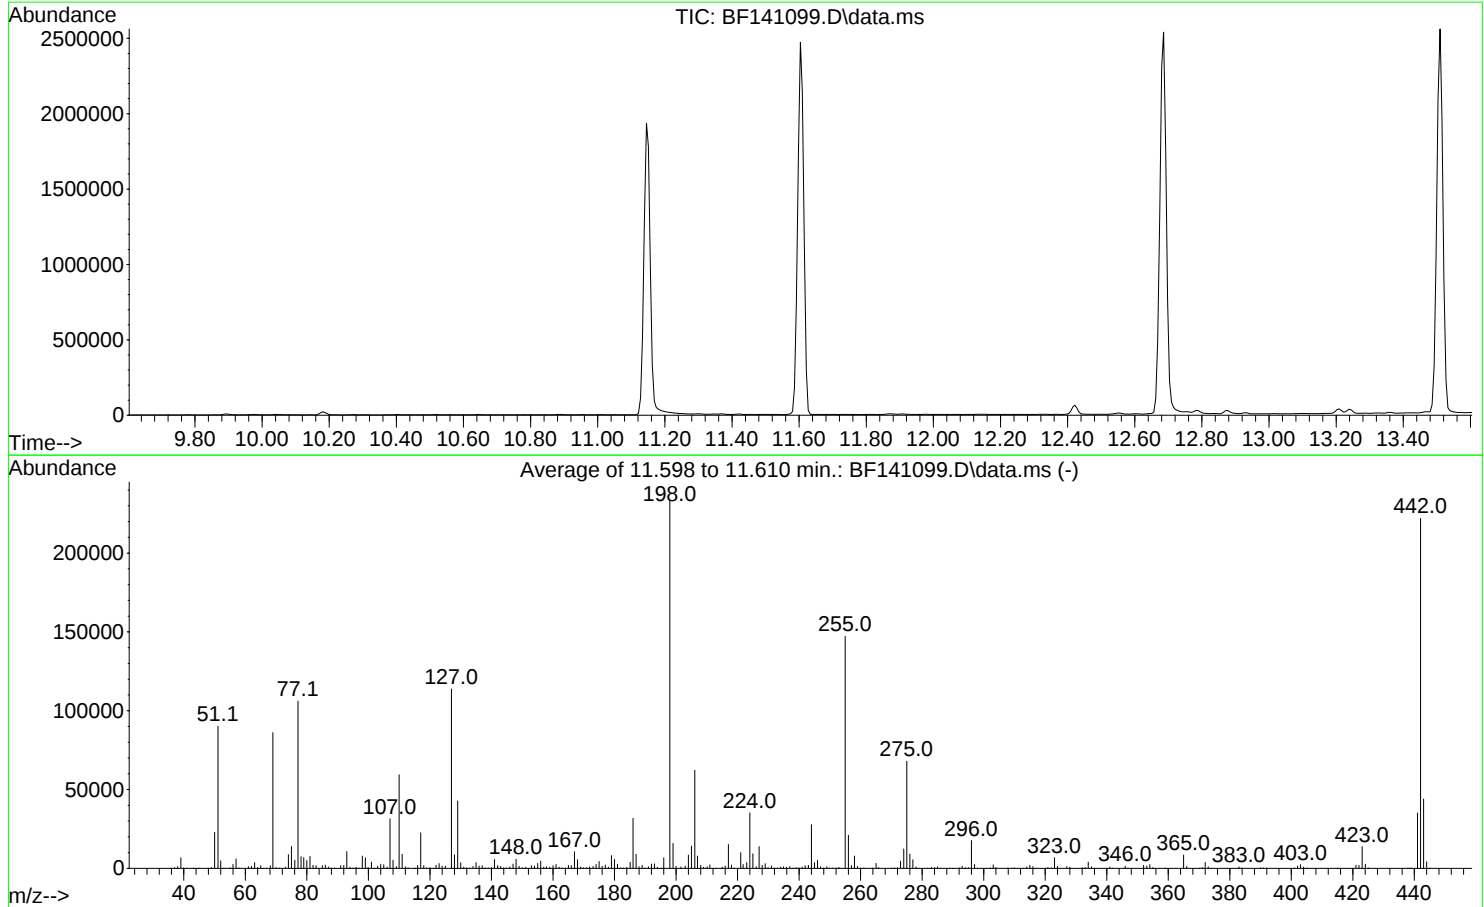

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	90293	PASS
68	69	0.00	2	1.9	1619	PASS
69	198	0.00	100	36.9	86073	PASS
70	69	0.00	2	0.6	556	PASS
127	198	10	80	48.8	113840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	233365	PASS
199	198	5	9	6.8	15797	PASS
275	198	10	60	29.1	67912	PASS
365	198	1	100	3.6	8406	PASS
441	198	0.01	100	15.0	35117	PASS
442	442	50	100	100.0	222016	PASS
443	442	15	24	19.8	43952	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
1/9/2025	BNA_F	<u>BF141099.D</u>
Compound Name	Response	Retention Time
DDT	635701	13.51
DDD	14907	13.21
DDE	5523	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20430	656131	3.11

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010925\
Data File : BF141099.D
Acq On : 09 Jan 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 09 12:03:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

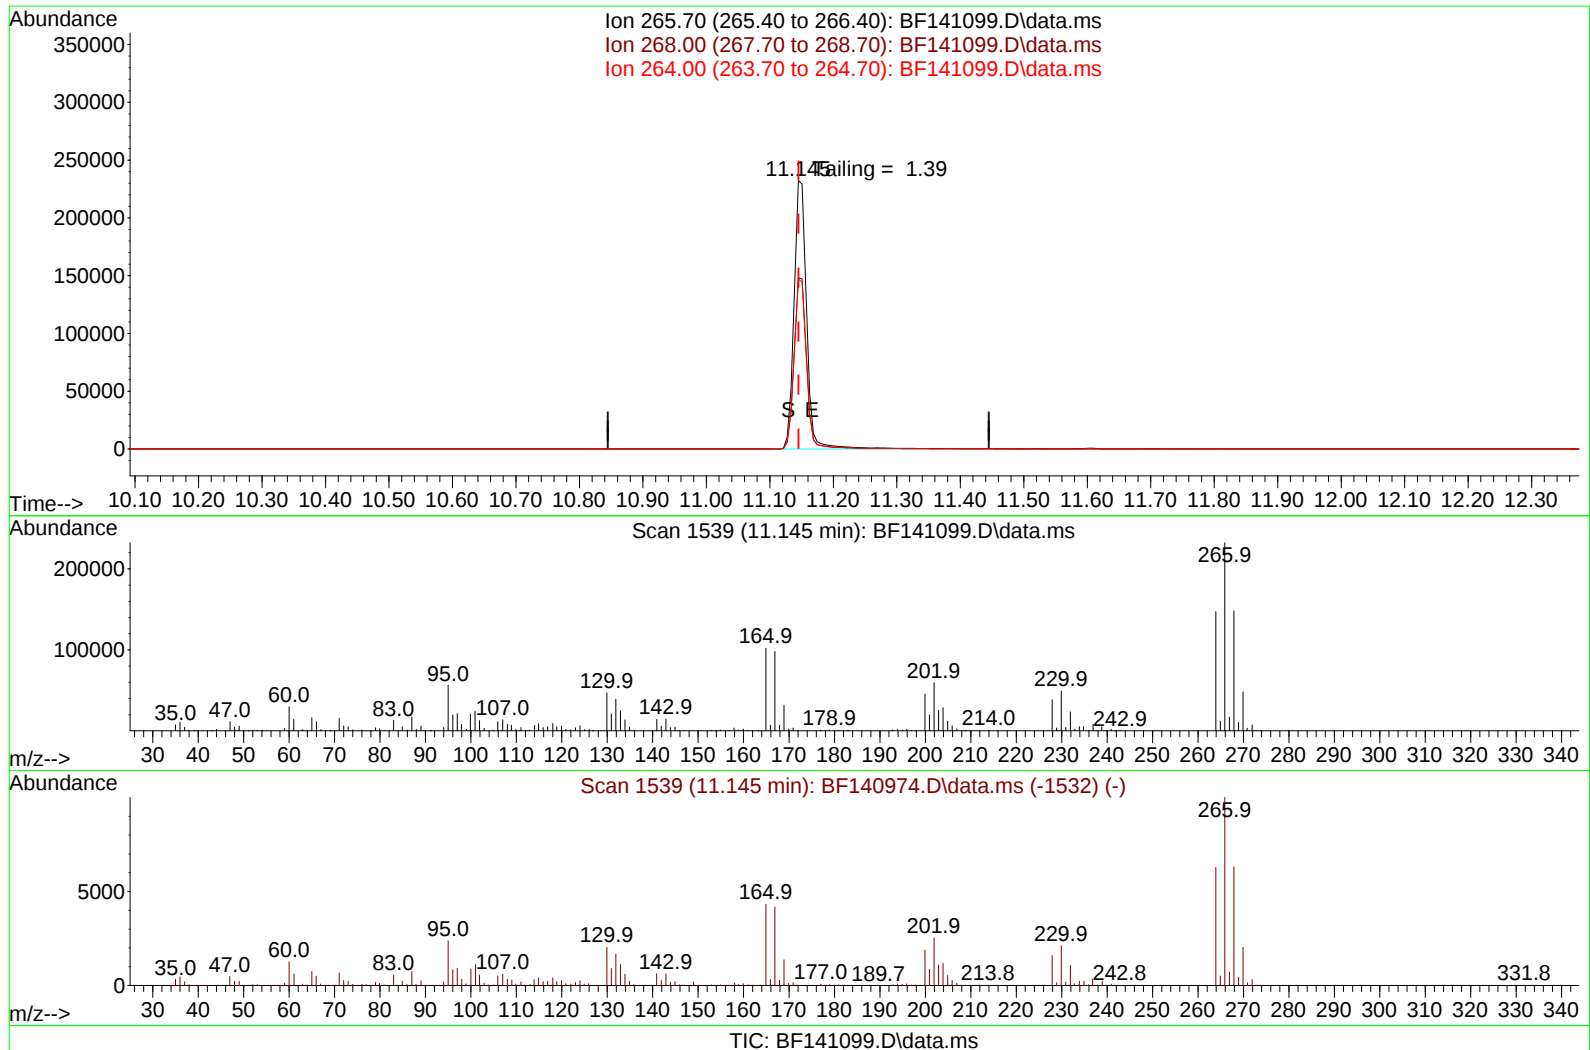

(70) Pentachlorophenol (C)

11.145min (0.000) 27821.83 ng




response 323344

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.74
264.00	62.80	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF010925\
Data File : BF141099.D
Acq On : 09 Jan 2025 10:38
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 09 12:03:34 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 27 00:31:16 2024
Response via : Initial Calibration

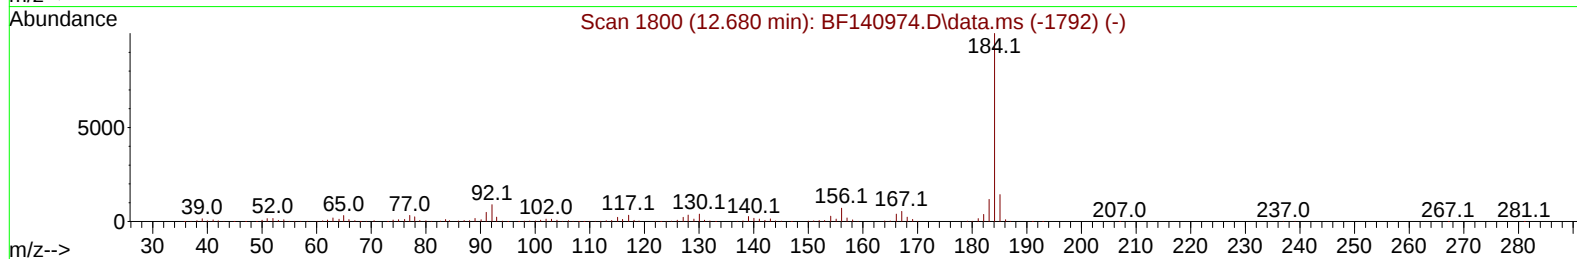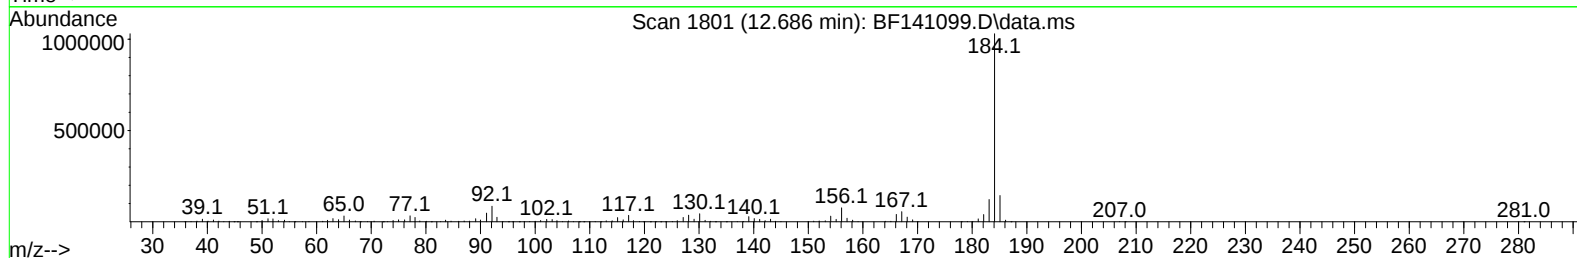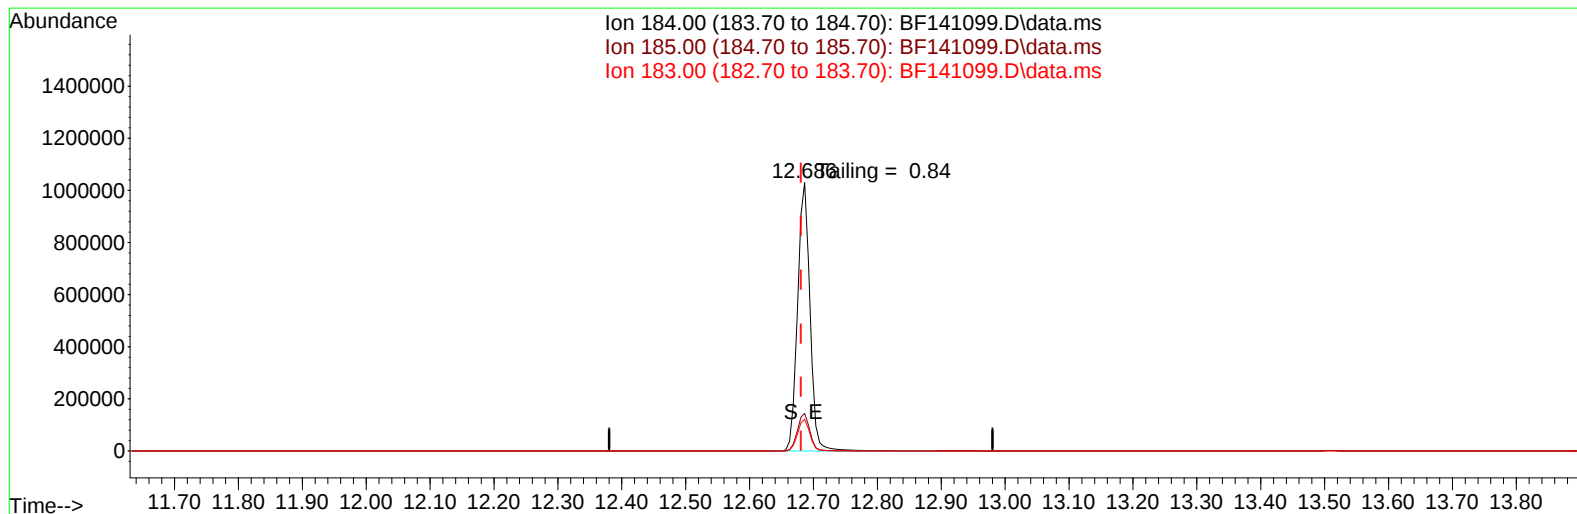

TIC: BF141099.D\data.ms

(77) Benzidine

12.686min (+ 0.006) 59252.02 ng

response 1399996

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.00
183.00	11.70	11.85
0.00	0.00	0.00