
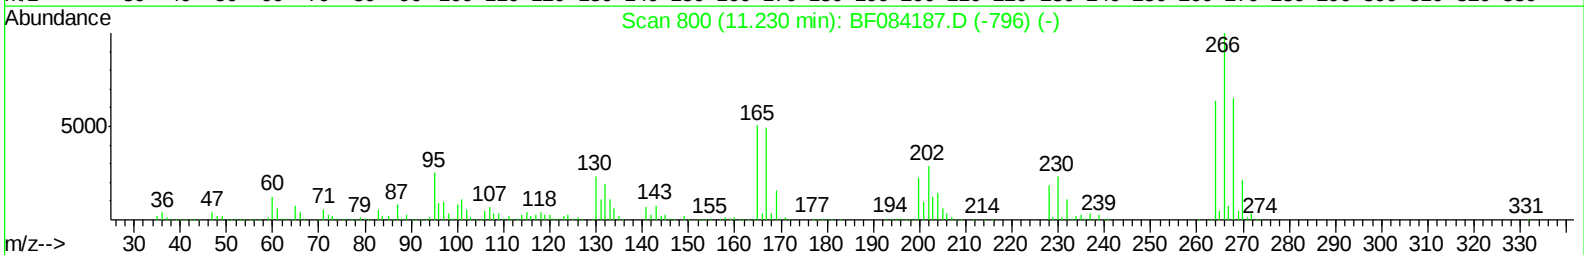
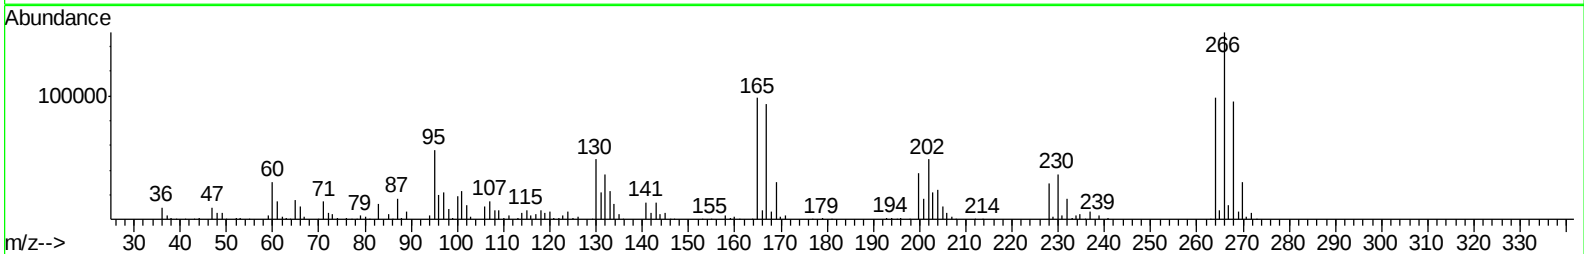


```
Data Path : Z:\HPCHEM1\BNA F\Data\BF011016\  
Data File : BF084350.D  
Acq On    : 10 Jan 2016    8:19  
Operator  : SJ/UM  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jan 11 06:55:01 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration



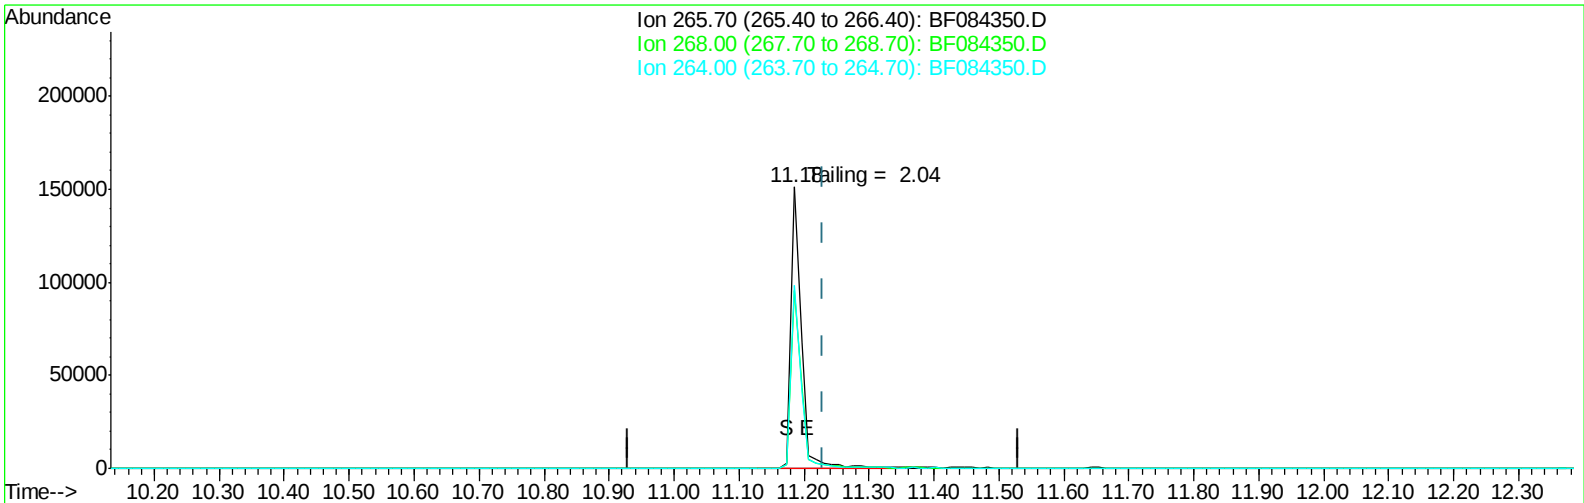


TIC: BF084350.D

(69) Pentachlorophenol (C)		
11.185min (-0.045) 43124.16ng		
response 171197		
Ion	Exp%	Act%
265.70	100	100
268.00	65.50	63.10
264.00	62.70	65.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF011016\
Data File : BF084350.D
Acq On : 10 Jan 2016 8:19
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 06:55:01 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

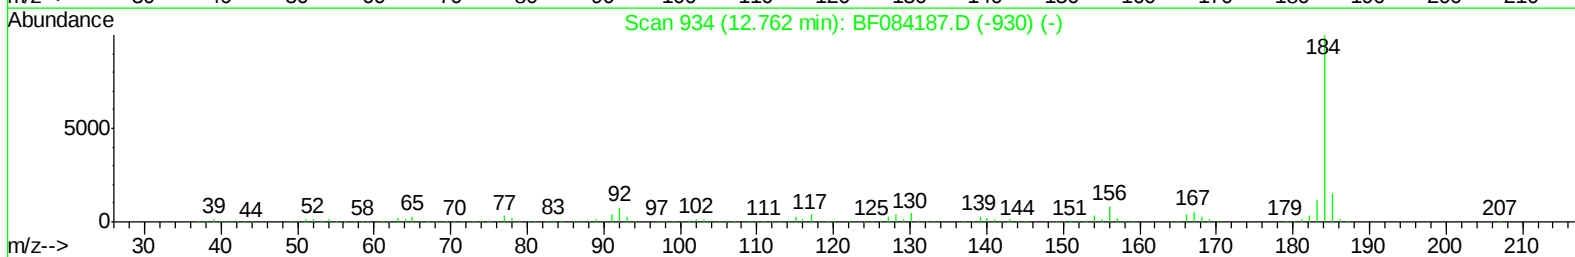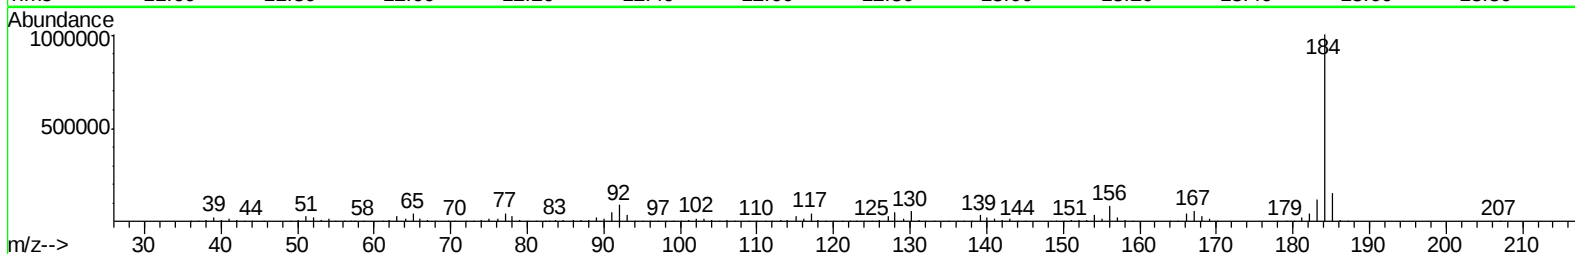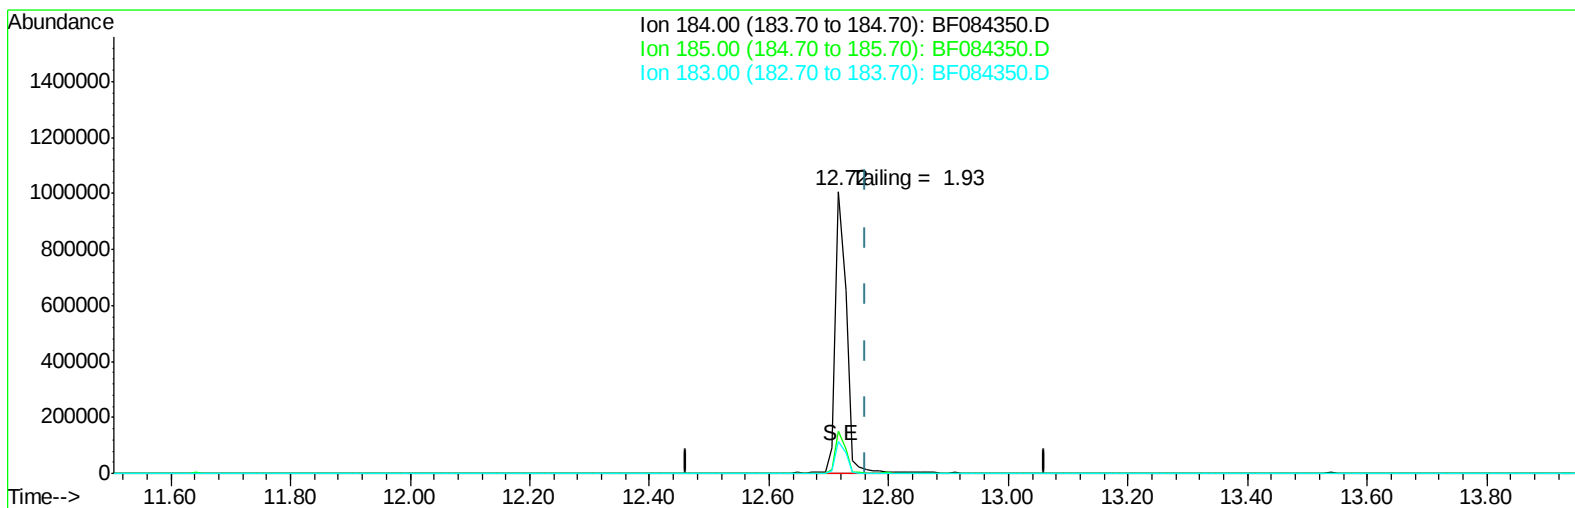

TIC: BF084350.D

(76) Benzidine

12.716min (-0.046) 9986.23ng

response 1309056

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.18
183.00	12.30	11.57
0.00	0.00	0.00