


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011016\
 Data File : BF084350.D
 Acq On : 10 Jan 2016 8:19
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

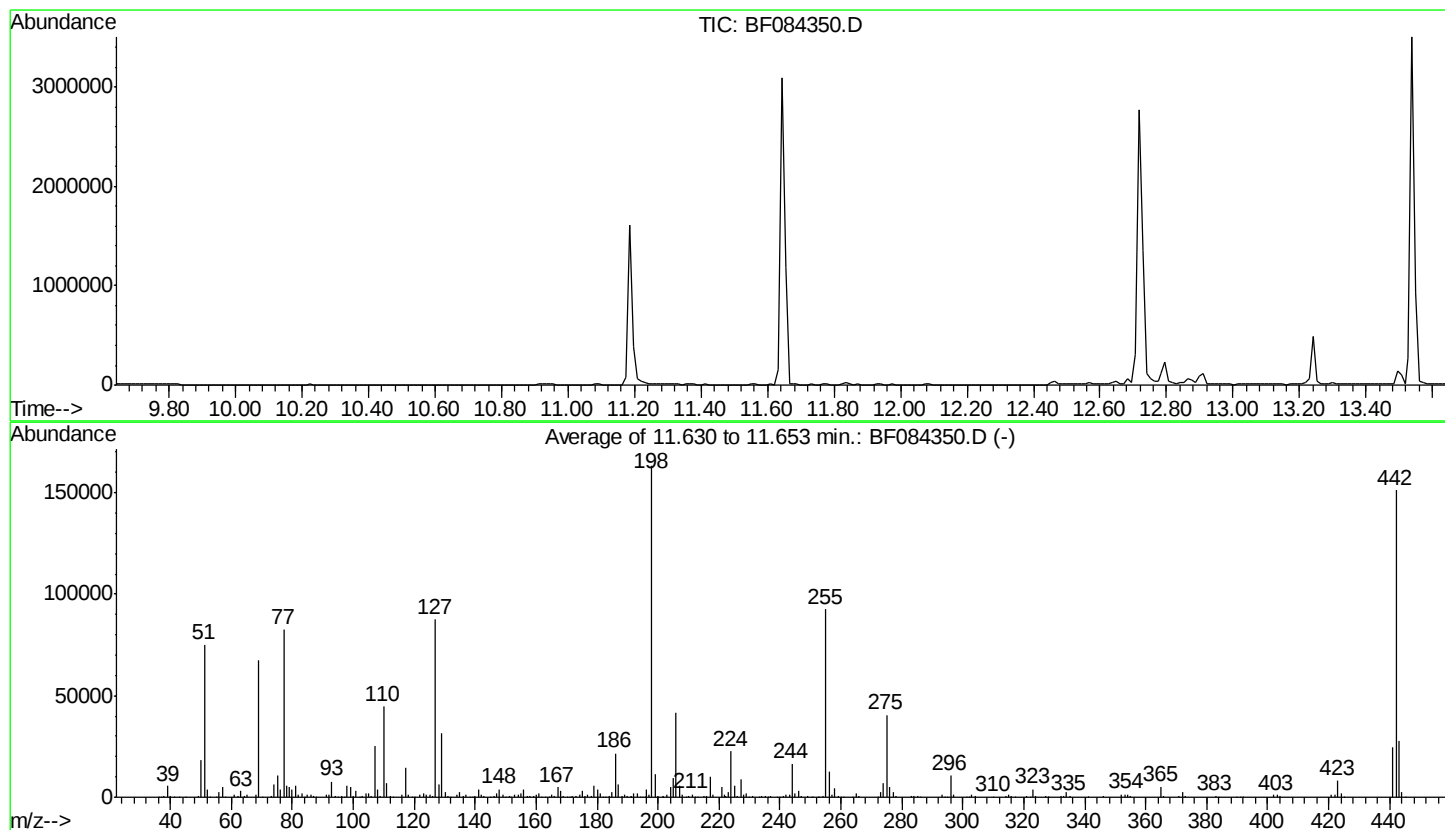

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	75157	PASS
68	69	0.00	2	1.8	1200	PASS
69	198	0.00	100	41.3	67504	PASS
70	69	0.00	2	0.5	314	PASS
127	198	10	80	53.6	87538	PASS
197	198	0.00	2	0.6	997	PASS
198	198	100	100	100.0	163334	PASS
199	198	5	9	6.9	11339	PASS
275	198	10	60	24.8	40494	PASS
365	198	1	100	3.1	5095	PASS
441	442	0.01	24	16.5	24877	PASS
442	198	50	100	92.5	151037	PASS
443	442	15	24	18.2	27525	PASS