


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011017\
 Data File : BF092173.D
 Acq On : 10 Jan 2017 11:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

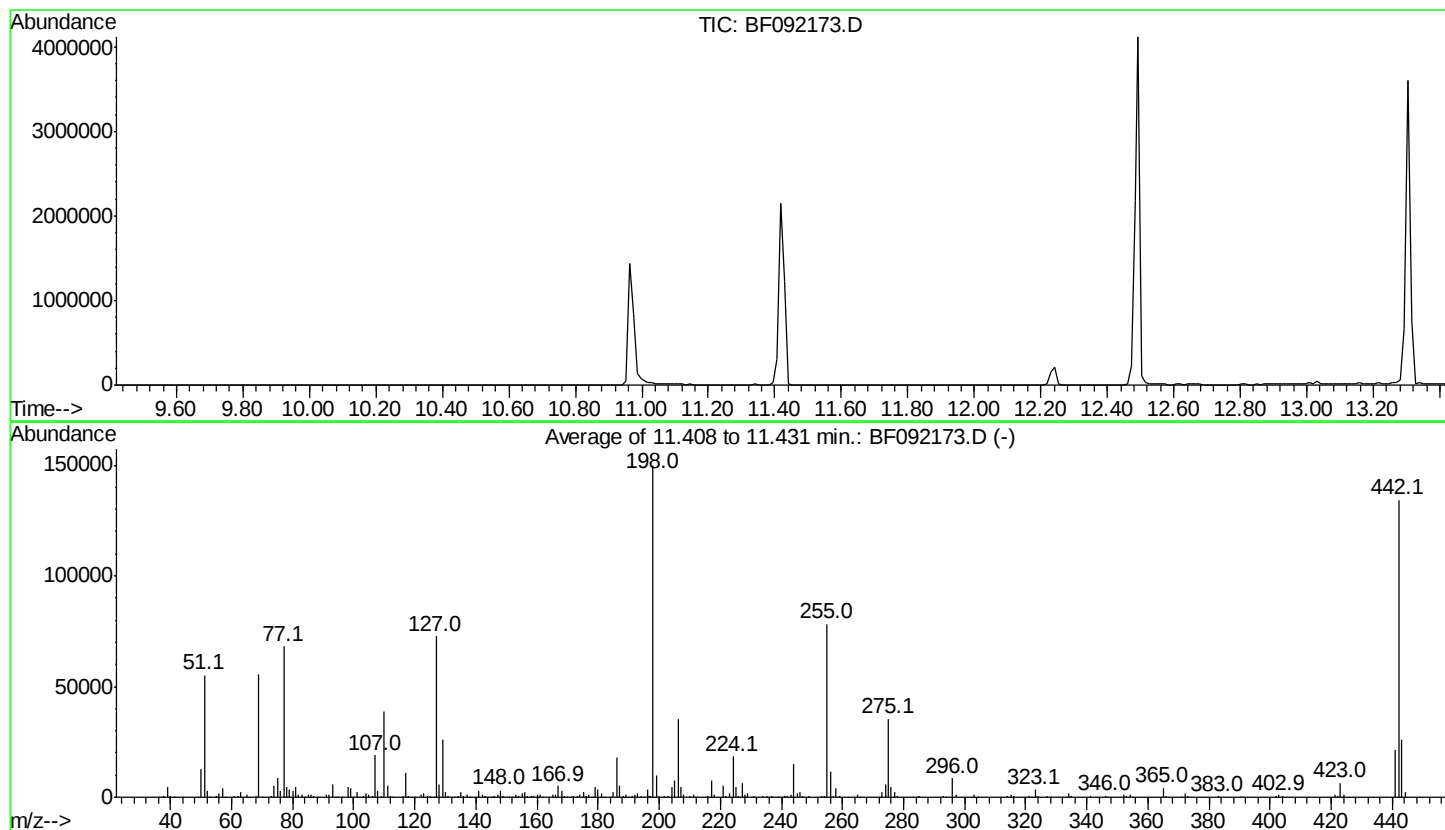

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	55027	PASS
68	69	0.00	2	1.3	697	PASS
69	198	0.00	100	37.0	55464	PASS
70	69	0.00	2	0.4	208	PASS
127	198	10	80	48.6	72768	PASS
197	198	0.00	2	0.5	726	PASS
198	198	100	100	100.0	149736	PASS
199	198	5	9	6.7	10027	PASS
275	198	10	60	23.7	35519	PASS
365	198	1	100	2.8	4190	PASS
441	442	0.01	24	16.1	21640	PASS
442	198	50	100	89.7	134246	PASS
443	442	15	24	19.4	25997	PASS