
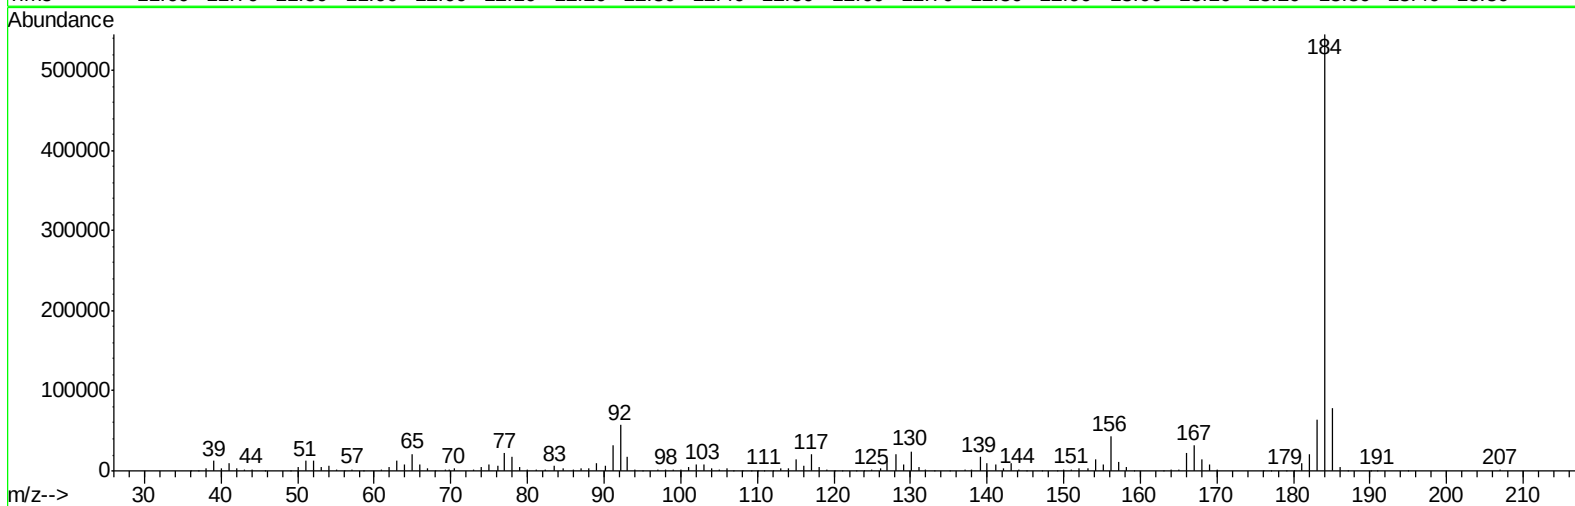


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011018\
Data File : BF101976.D
Acq On : 10 Jan 2018 13:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 06:41:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 15:20:36 2018
Response via : Initial Calibration

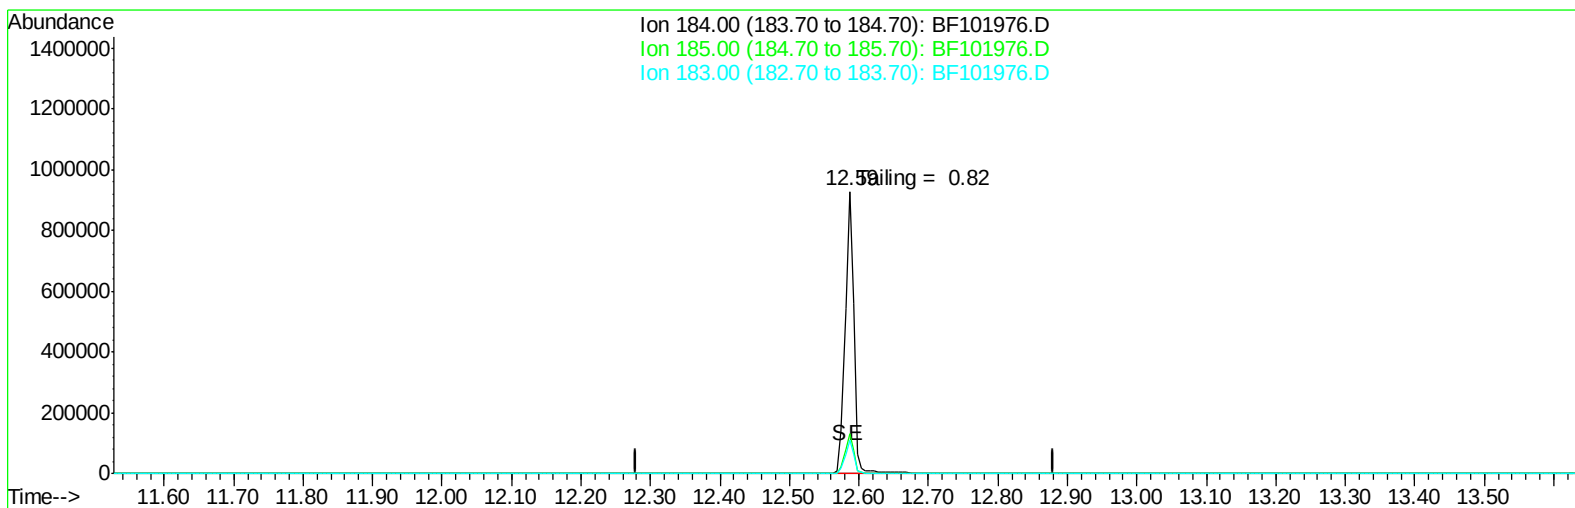

TIC: BF101976.D

(76) Benzidine



12.580min (-12.580) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	15.70	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011018\
Data File : BF101976.D
Acq On : 10 Jan 2018 13:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 06:41:06 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 15:20:36 2018
Response via : Initial Calibration

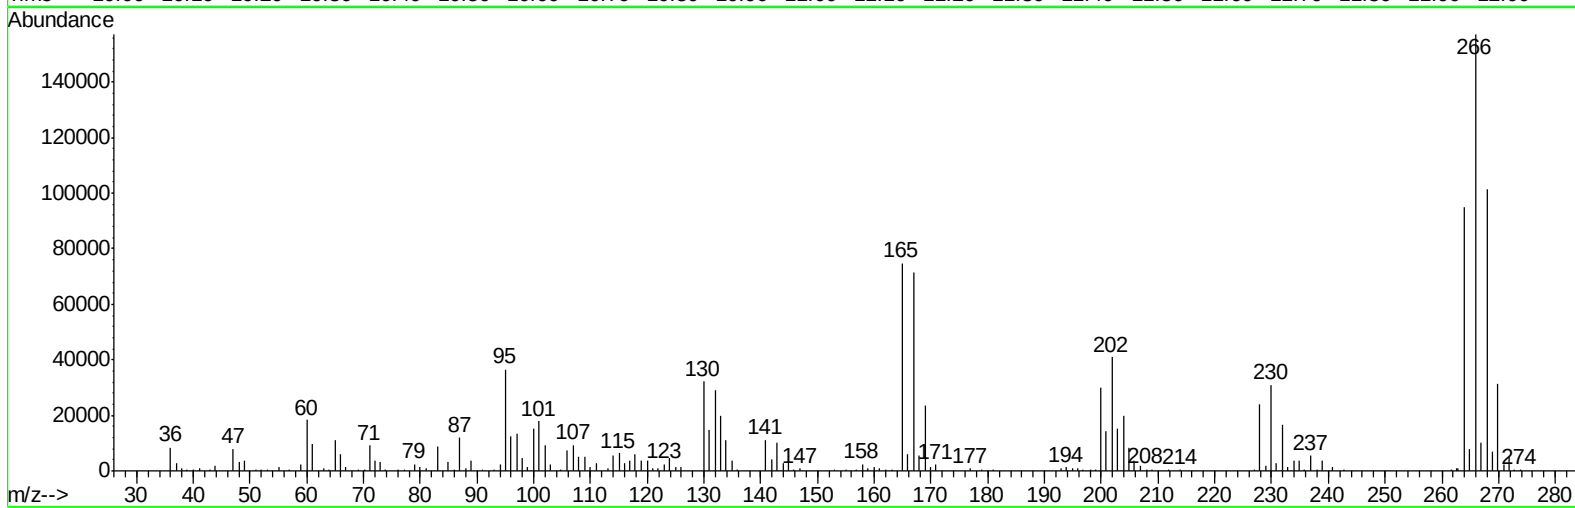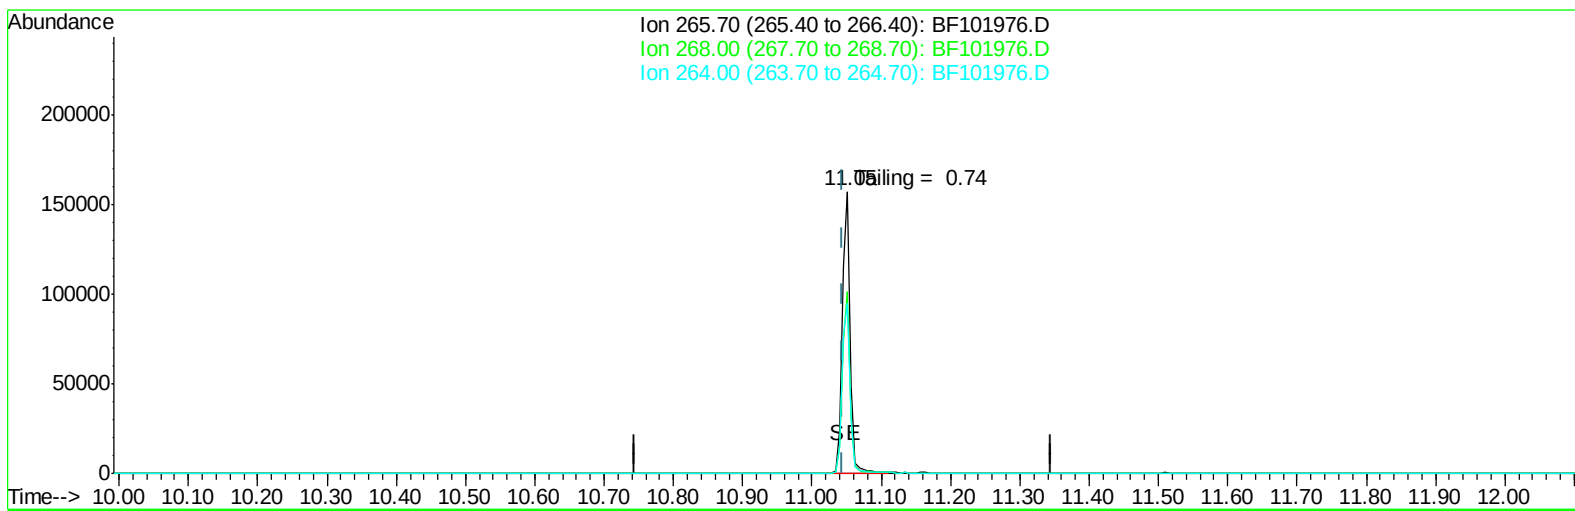

TIC: BF101976.D

(69) Pentachlorophenol (C)

11.051min (+0.006) 48632.36ng

response 128209

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.45
264.00	61.90	60.31
0.00	0.00	0.00