
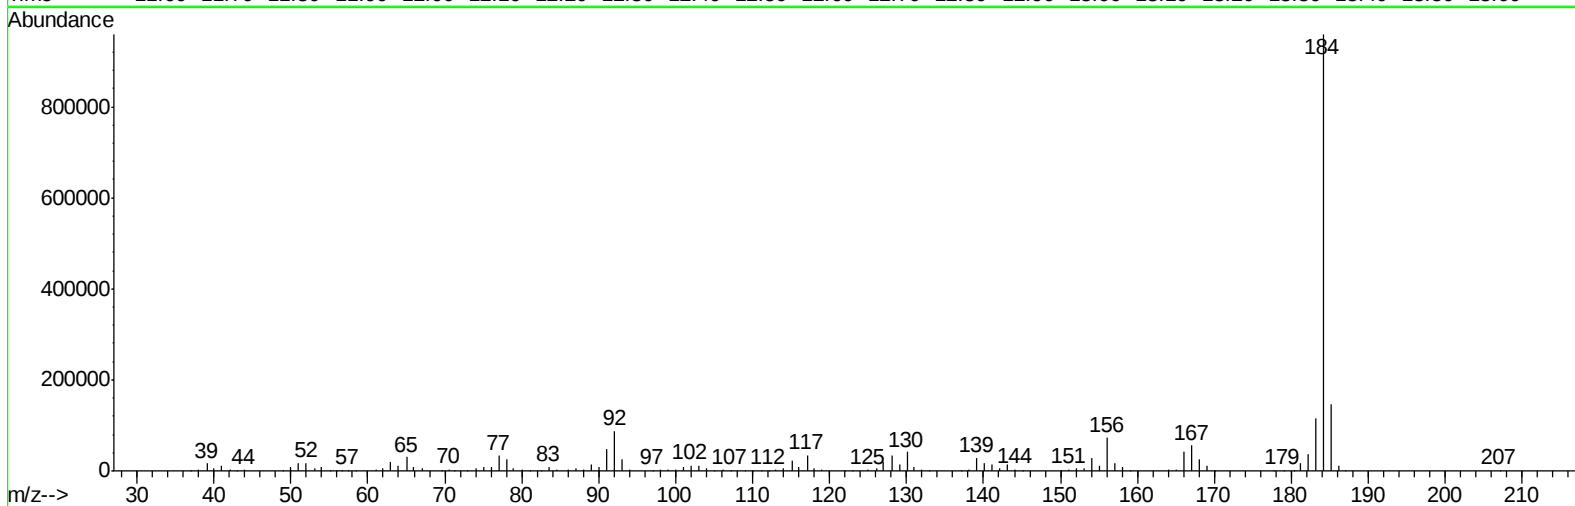


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011018\
Data File : BF101980.D
Acq On : 10 Jan 2018 15:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 06:42:03 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 15:20:36 2018
Response via : Initial Calibration

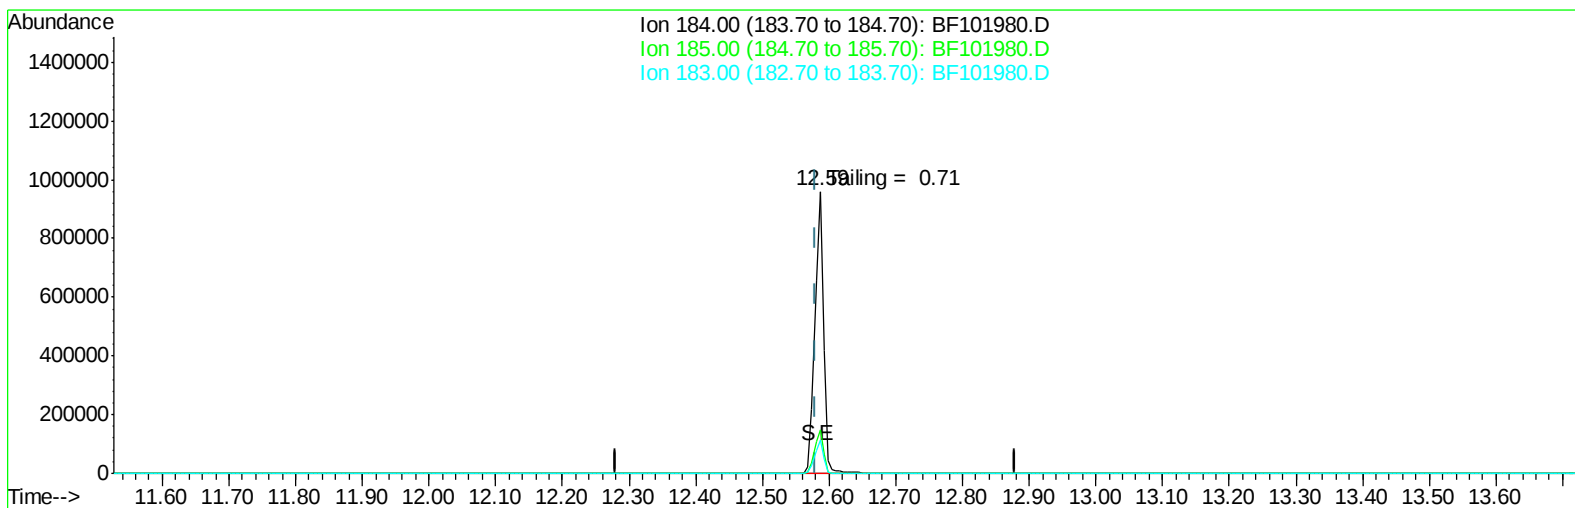

TIC: BF101980.D

(76) Benzidine



12.586min (+0.006) 150310.46ng

response 841964

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.38
183.00	11.60	11.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF011018\
Data File : BF101980.D
Acq On : 10 Jan 2018 15:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 06:42:03 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 15:20:36 2018
Response via : Initial Calibration

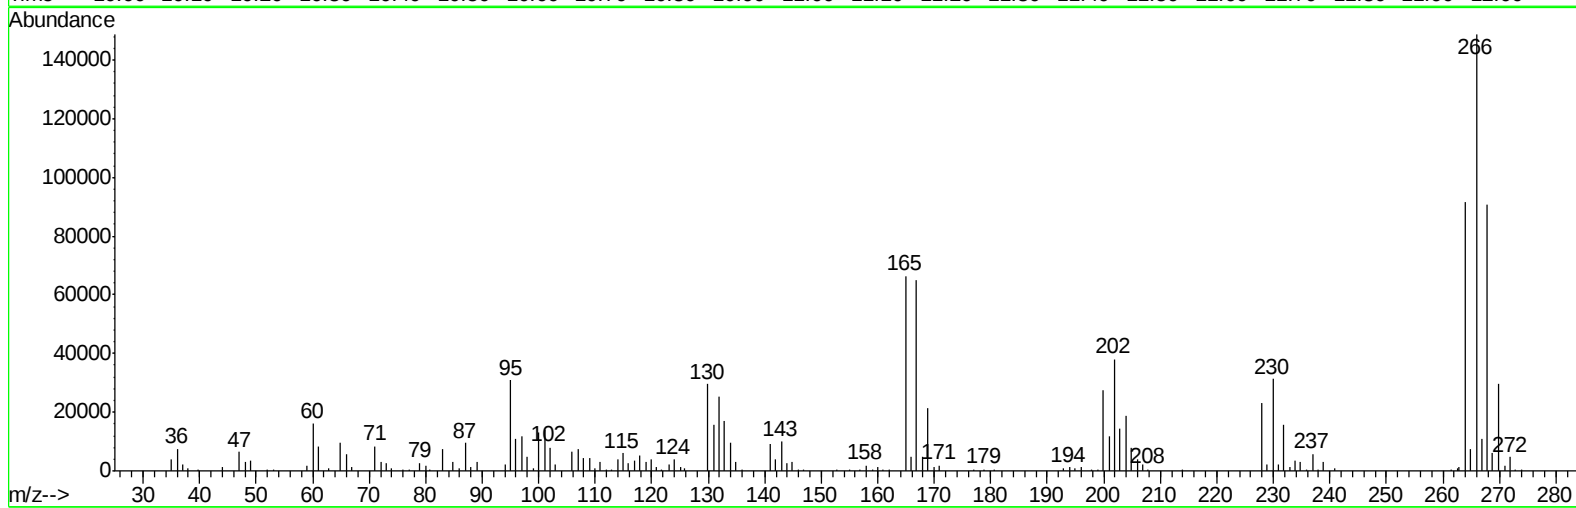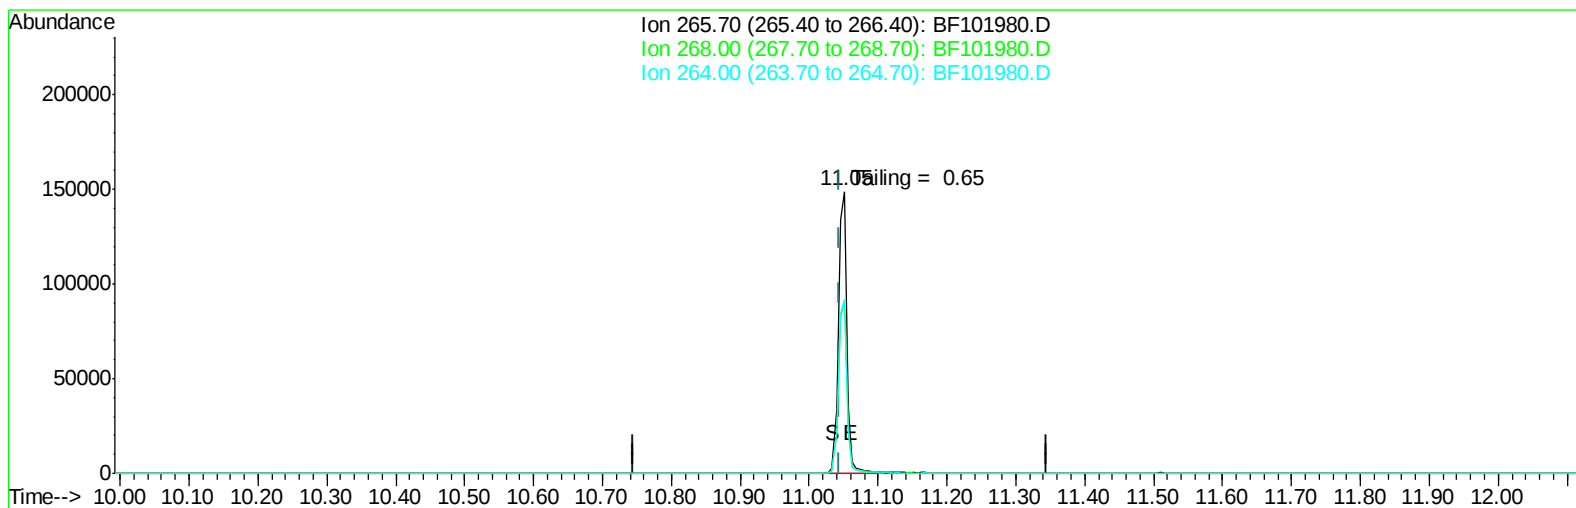

TIC: BF101980.D

(69) Pentachlorophenol (C)

11.051min (+0.006) 151931.93ng

response 131376

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.14
264.00	61.90	61.64
0.00	0.00	0.00