

Data Path : U:\HPCHEM1\BNA F\DATA\BF011018\
 Data File : BF102002.D
 Acq On : 11 Jan 2018 1:43
 Operator : SJ/JU
 Sample : J1076-17 50X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-52-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.322	547	550	553	rVB	19458	18750	1.03%	0.146%
2	6.345	722	724	729	rBV2	22675	20634	1.13%	0.161%
3	6.728	785	789	792	rBV	1438552	1254509	68.79%	9.798%
4	6.904	816	819	822	rVB	71304	53574	2.94%	0.418%
5	6.987	829	833	836	rBV	25879	24425	1.34%	0.191%
6	8.010	1002	1007	1009	rBV	1821000	1823805	100.00%	14.244%
7	8.028	1009	1010	1013	rVV	1004011	578610	31.73%	4.519%
8	8.081	1013	1019	1022	rVB	28710	27348	1.50%	0.214%
9	8.716	1123	1127	1131	rBV	113858	98250	5.39%	0.767%
10	8.816	1138	1144	1147	rBV	115980	88253	4.84%	0.689%
11	9.081	1184	1189	1192	rVB	24107	20581	1.13%	0.161%
12	9.180	1203	1206	1211	rVB	21916	19804	1.09%	0.155%
13	9.345	1231	1234	1238	rBV2	27464	36954	2.03%	0.289%
14	9.416	1243	1246	1249	rBV	42013	40903	2.24%	0.319%
15	9.622	1277	1281	1285	rBV	90621	86515	4.74%	0.676%
16	9.757	1298	1304	1308	rBV	1681663	1613945	88.49%	12.605%
17	9.792	1308	1310	1314	rVB	115871	95649	5.24%	0.747%
18	9.963	1335	1339	1342	rBV	117024	97729	5.36%	0.763%
19	10.163	1370	1373	1375	rBV3	19006	20163	1.11%	0.157%
20	10.304	1394	1397	1403	rVB	206846	165805	9.09%	1.295%
21	10.463	1421	1424	1427	rVB	24233	22029	1.21%	0.172%
22	10.539	1433	1437	1442	rVB3	32622	43208	2.37%	0.337%
23	10.675	1457	1460	1464	rVB3	27057	36187	1.98%	0.283%
24	10.851	1486	1490	1493	rBV2	30039	32332	1.77%	0.253%
25	11.139	1533	1539	1544	rBV3	72681	86104	4.72%	0.672%
26	11.239	1553	1556	1559	rBV	1471642	1438404	78.87%	11.234%
27	11.263	1559	1560	1564	rVV	662840	400324	21.95%	3.127%
28	11.316	1564	1569	1572	rVB	166009	142591	7.82%	1.114%
29	11.351	1572	1575	1578	rBV4	14391	21692	1.19%	0.169%
30	11.469	1593	1595	1598	rBV	32278	29645	1.63%	0.232%
31	11.569	1610	1612	1618	rVB3	27735	30939	1.70%	0.242%
32	11.657	1624	1627	1631	rVB2	20244	24096	1.32%	0.188%
33	11.739	1639	1641	1643	rVV	60687	44654	2.45%	0.349%
34	11.769	1643	1646	1649	rVB	86346	77374	4.24%	0.604%

Data Path : U:\HPCHEM1\BNA_F\DATA\BF011018\
 Data File : BF102002.D
 Acq On : 11 Jan 2018 1:43
 Operator : SJ/JU
 Sample : J1076-17 50X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-52-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.816	1651	1654	1656	rBV	30161	26420	1.45%	0.206%
36	11.851	1657	1660	1663	rBV	129092	125249	6.87%	0.978%
37	11.921	1669	1672	1675	rBV5	18273	23677	1.30%	0.185%
38	12.039	1689	1692	1694	rBV	35694	36157	1.98%	0.282%
39	12.163	1711	1713	1715	rBV3	15764	18296	1.00%	0.143%
40	12.221	1720	1723	1724	rBV2	28258	34485	1.89%	0.269%
41	12.292	1732	1735	1738	rBV3	40891	45780	2.51%	0.358%
42	12.451	1758	1762	1765	rBV	410318	377337	20.69%	2.947%
43	12.545	1775	1778	1781	rBV	52910	50922	2.79%	0.398%
44	12.674	1795	1800	1804	rBV	358026	338677	18.57%	2.645%
45	12.821	1823	1825	1833	rVB3	49882	57060	3.13%	0.446%
46	13.004	1854	1856	1860	rVB	81903	64222	3.52%	0.502%
47	13.068	1865	1867	1870	rVV	54018	47858	2.62%	0.374%
48	13.110	1871	1874	1876	rVV2	52950	57034	3.13%	0.445%
49	13.874	1999	2004	2007	rBV	1083849	1142033	62.62%	8.919%
50	13.898	2007	2008	2011	rVB	148527	74912	4.11%	0.585%
51	14.886	2172	2176	2179	rBV	116730	190902	10.47%	1.491%
52	15.174	2222	2225	2228	rVB	70864	71940	3.94%	0.562%
53	15.227	2231	2234	2239	rVB	140450	151800	8.32%	1.186%
54	15.292	2240	2245	2249	rBV	896041	1041585	57.11%	8.135%
55	16.656	2473	2477	2483	rVB2	59364	106975	5.87%	0.835%
56	17.068	2544	2547	2552	rVB	39807	61006	3.34%	0.476%
57	19.033	2874	2881	2882	rBV7	26205	44014	2.41%	0.344%


Sum of corrected areas: 12804126

Data Path : U:\HPCHEM1\BNA F\DATA\BF011018\
Data File : BF102002.D
Acq On : 11 Jan 2018 1:43
Operator : SJ/JU
Sample : J1076-17 50X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-52-01

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

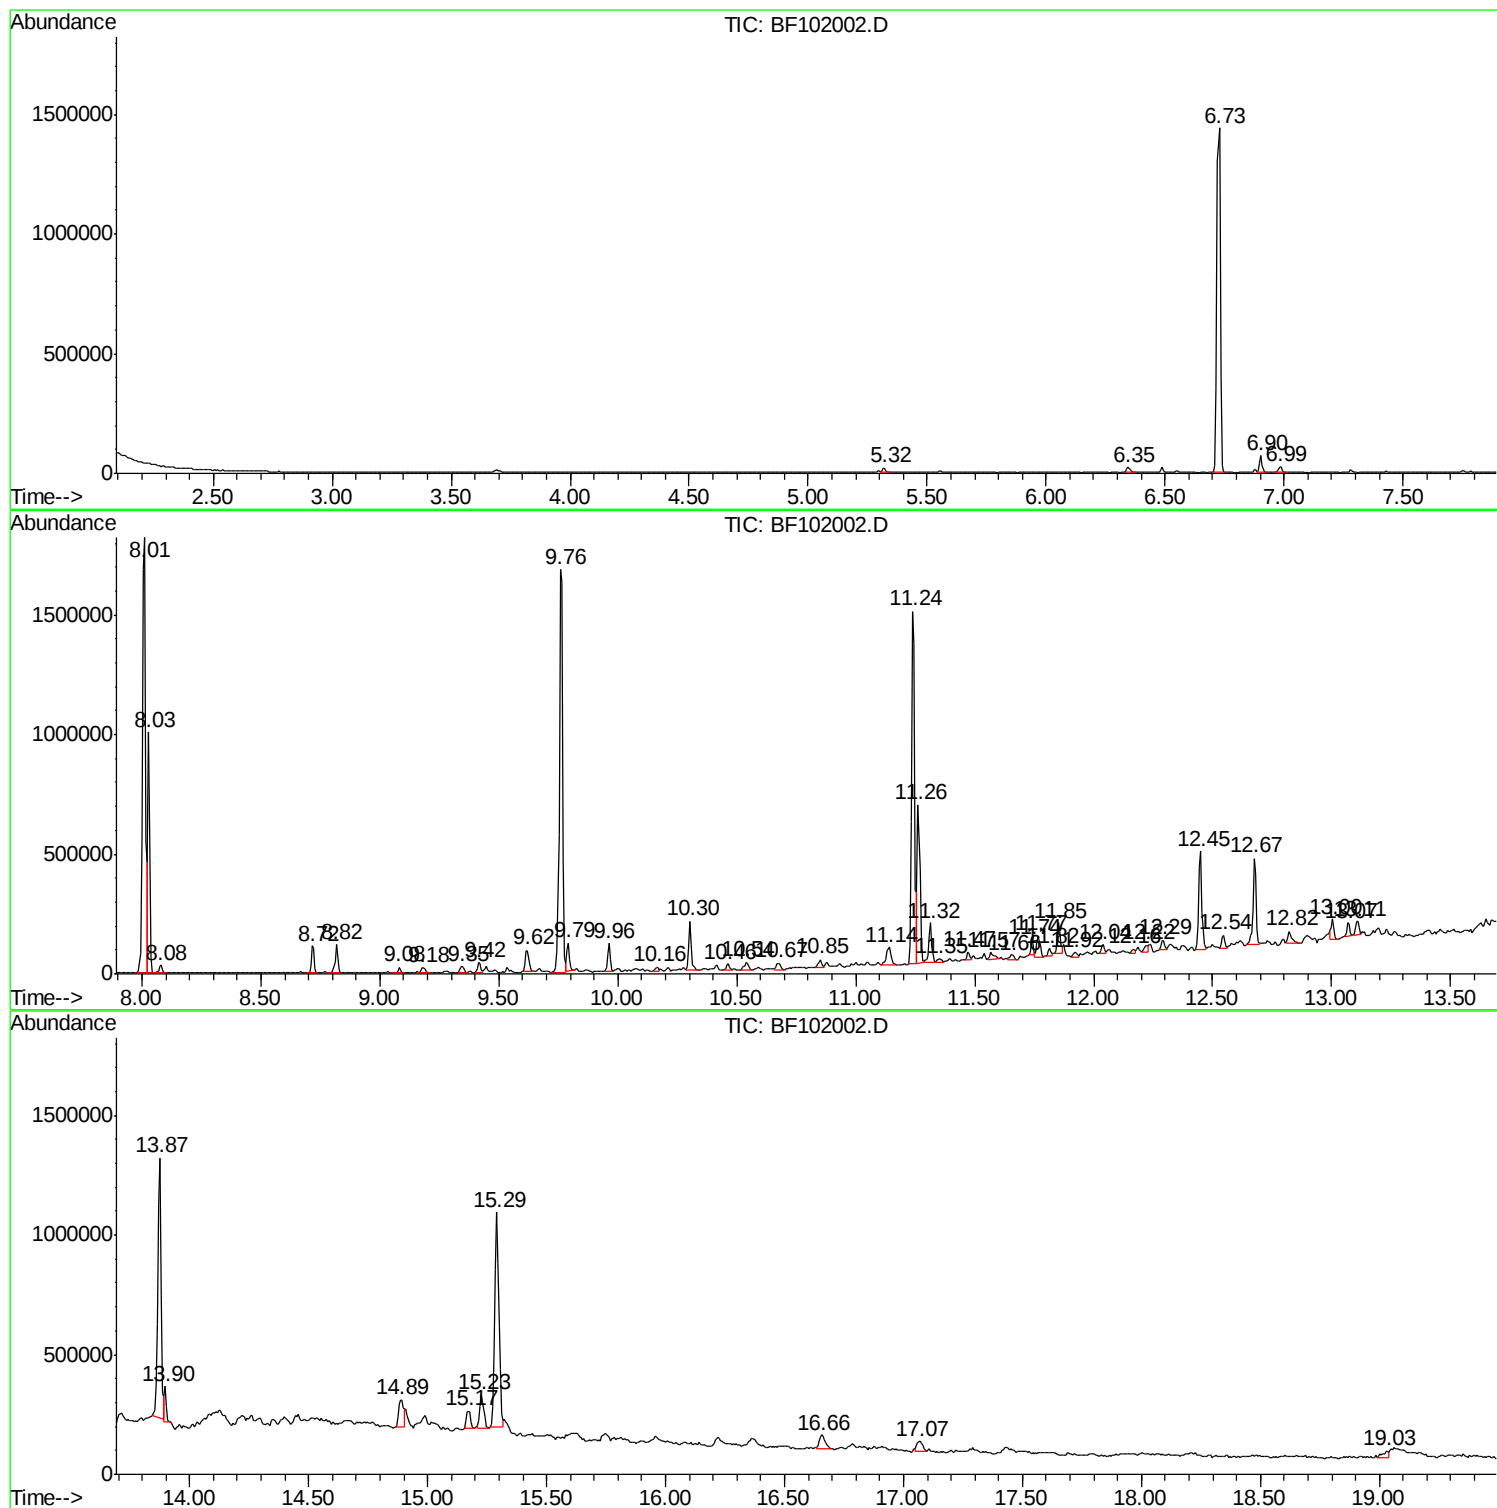

Data_Path : U:\HPCHEM1\BNA_F\DATA\BF011018\
Data_File : BF102002.D
Acq_On : 11-Jan-2018 1:433
Operator : SJ/JUU
Sample : J1076-17.50XX
Misc :
ALS_Vial : 23 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
WC-52-01

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
