


Data Path : U:\HPCHEM1\BNA F\Data\BF011018\
 Data File : BF101976.D
 Acq On : 10 Jan 2018 13:08
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 09 15:20:36 2018

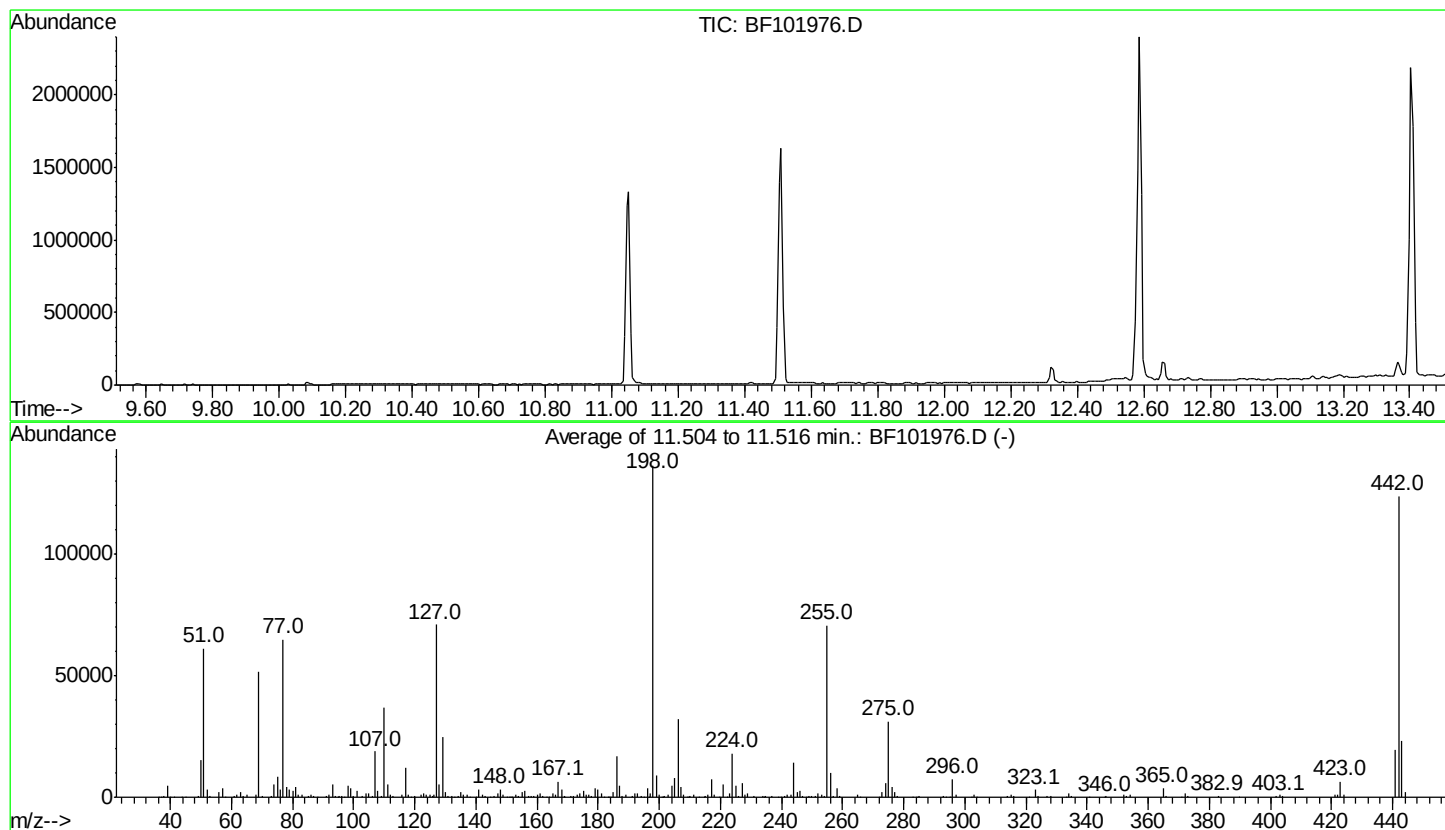

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	61235	PASS
68	69	0.00	2	1.8	930	PASS
69	198	0.00	100	38.0	51782	PASS
70	69	0.00	2	0.6	310	PASS
127	198	10	80	52.1	70877	PASS
197	198	0.00	2	1.0	1414	PASS
198	198	100	100	100.0	136130	PASS
199	198	5	9	6.7	9153	PASS
275	198	10	60	22.8	31026	PASS
365	198	1	100	2.9	3881	PASS
441	443	0.01	100	83.0	19210	PASS
442	198	50	100	90.9	123770	PASS
443	442	15	24	18.7	23133	PASS