


Data Path : U:\HPCHEM1\BNA_F\Data\BF011018\
 Data File : BF101980.D
 Acq On : 10 Jan 2018 15:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF010918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 09 15:20:36 2018

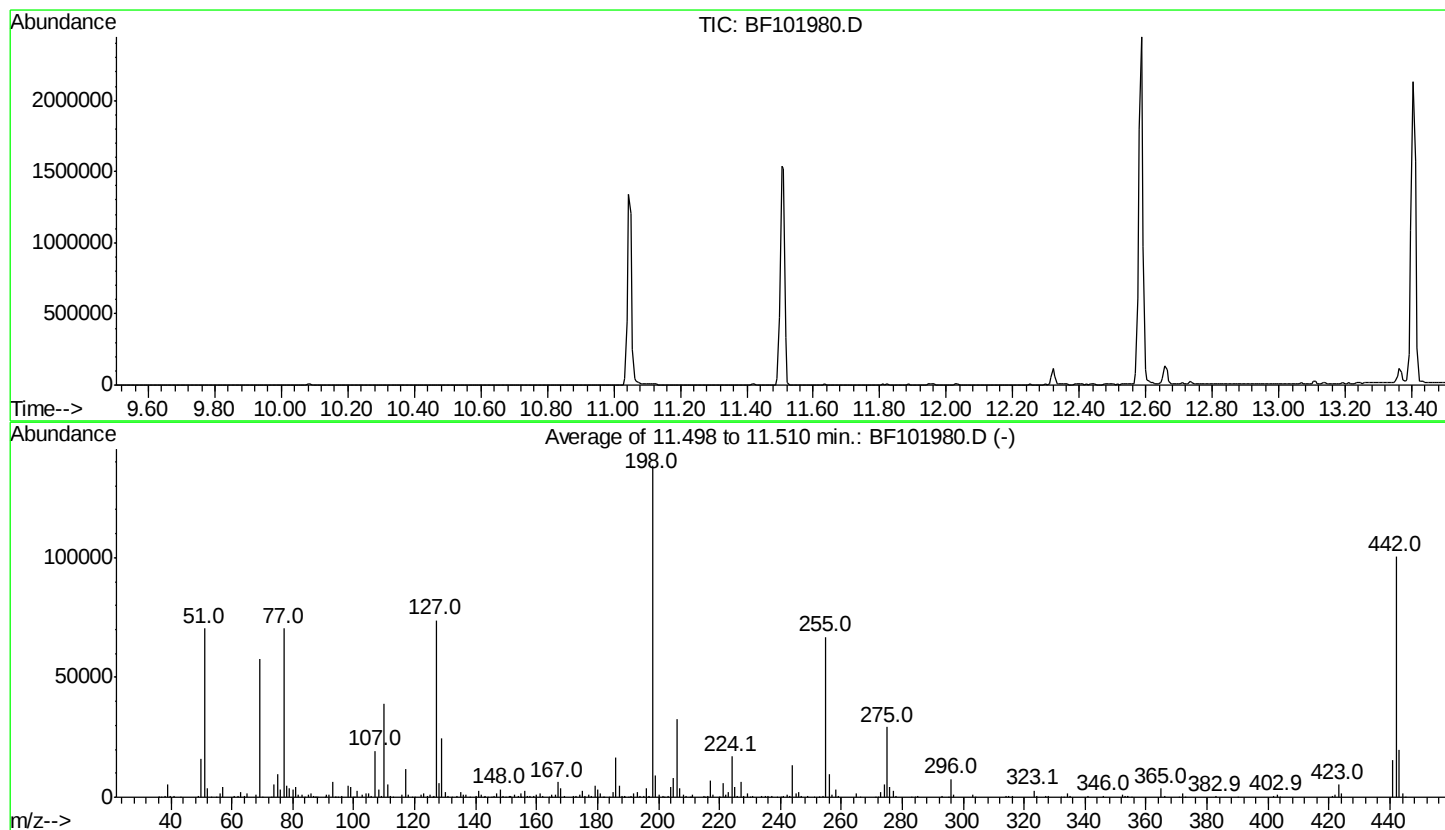

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	70480	PASS
68	69	0.00	2	1.9	1094	PASS
69	198	0.00	100	41.5	57485	PASS
70	69	0.00	2	0.4	228	PASS
127	198	10	80	53.4	73882	PASS
197	198	0.00	2	0.5	677	PASS
198	198	100	100	100.0	138445	PASS
199	198	5	9	6.6	9198	PASS
275	198	10	60	21.2	29284	PASS
365	198	1	100	2.6	3553	PASS
441	443	0.01	100	78.7	15721	PASS
442	198	50	100	72.4	100269	PASS
443	442	15	24	19.9	19964	PASS