

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011022\
 Data File : BF126581.D
 Acq On : 10 Jan 2022 21:54
 Operator : JU/CG
 Sample : N1076-04 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-04

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126581.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.769	280	286	290	rBB	7171	9920	1.61%	0.264%
2	5.375	556	559	569	rVB	151231	144050	23.31%	3.835%
3	6.398	730	733	742	rBV	169475	144715	23.42%	3.853%
4	6.769	792	796	800	rBV	615747	488659	79.07%	13.011%
5	7.328	888	891	897	rVB	110551	84736	13.71%	2.256%
6	8.051	1010	1014	1018	rBV	749744	618000	100.00%	16.455%
7	9.127	1194	1197	1201	rBV	183572	135072	21.86%	3.596%
8	9.810	1309	1313	1316	rBV	702743	554108	89.66%	14.753%
9	10.592	1444	1446	1451	rBB	61141	55196	8.93%	1.470%
10	11.298	1562	1566	1569	rBV	549207	495126	80.12%	13.183%
11	12.510	1767	1772	1776	rBV	8448	7898	1.28%	0.210%
12	12.880	1832	1835	1839	rVB	144708	116601	18.87%	3.105%
13	13.939	2011	2015	2019	rBV	531244	461640	74.70%	12.291%
14	14.039	2028	2032	2037	rBV	73186	72129	11.67%	1.920%
15	15.392	2257	2262	2267	rBV2	299598	367942	59.54%	9.797%




Sum of corrected areas: 3755792

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011022\
Data File : BF126581.D
Acq On : 10 Jan 2022 21:54
Operator : JU/CG
Sample : N1076-04 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

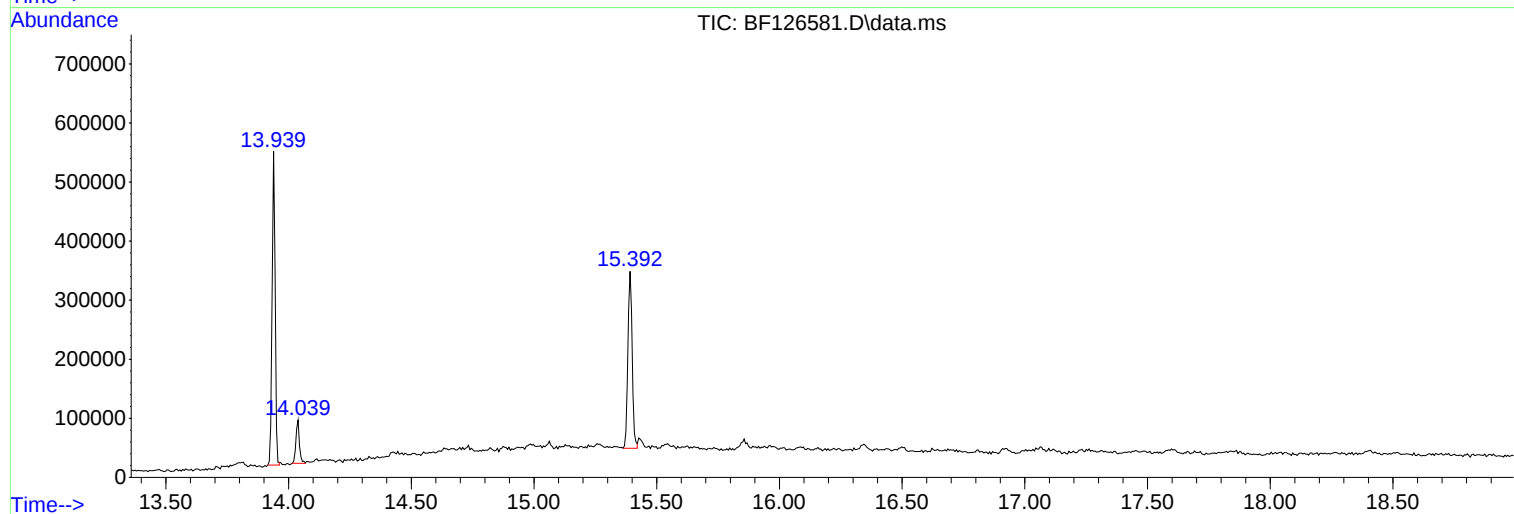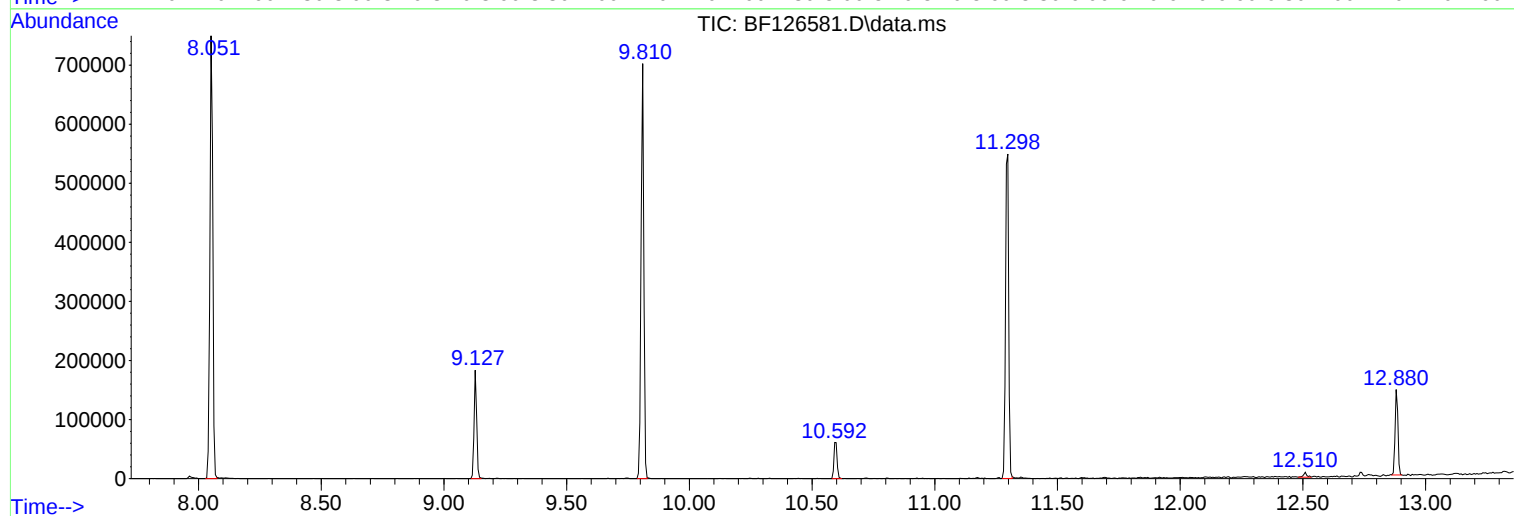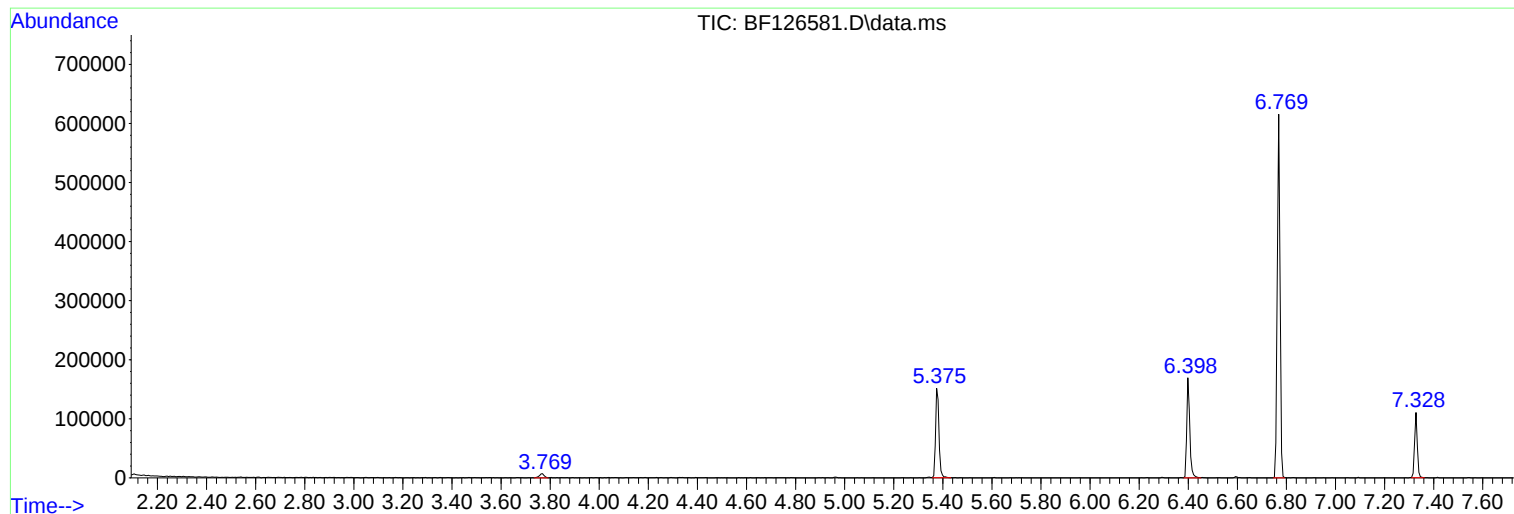

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011022\
Data File : BF126581.D
Acq On : 10 Jan 2022 21:54
Operator : JU/CG
Sample : N1076-04 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-04










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.039	3.12 ng	72129	Chrysene-d12	13.939

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	64
3			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19N03S	1000483-83-4	58
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	53
5			Cobalt, (.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	42

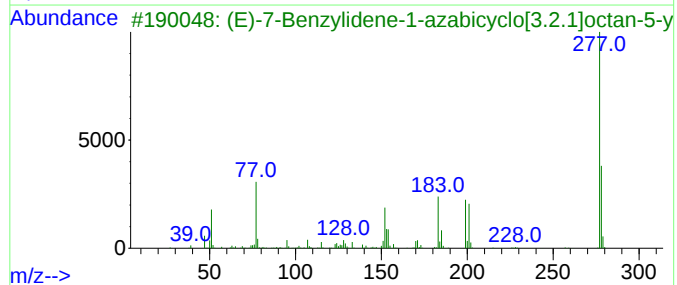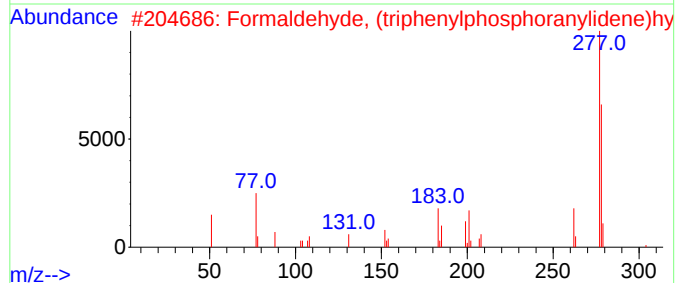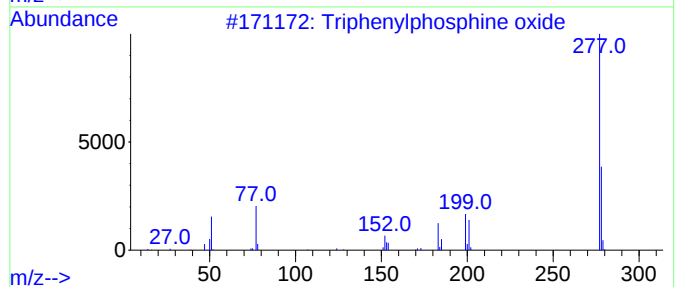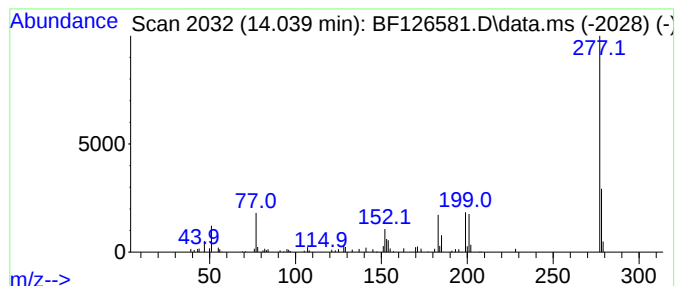

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011022\
Data File : BF126581.D
Acq On : 10 Jan 2022 21:54
Operator : JU/CG
Sample : N1076-04 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-04

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.039	3.1	ng	72129	5	13.939	461640	20.0