


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011022\
 Data File : BF126558.D
 Acq On : 10 Jan 2022 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 10 14:50:31 2022

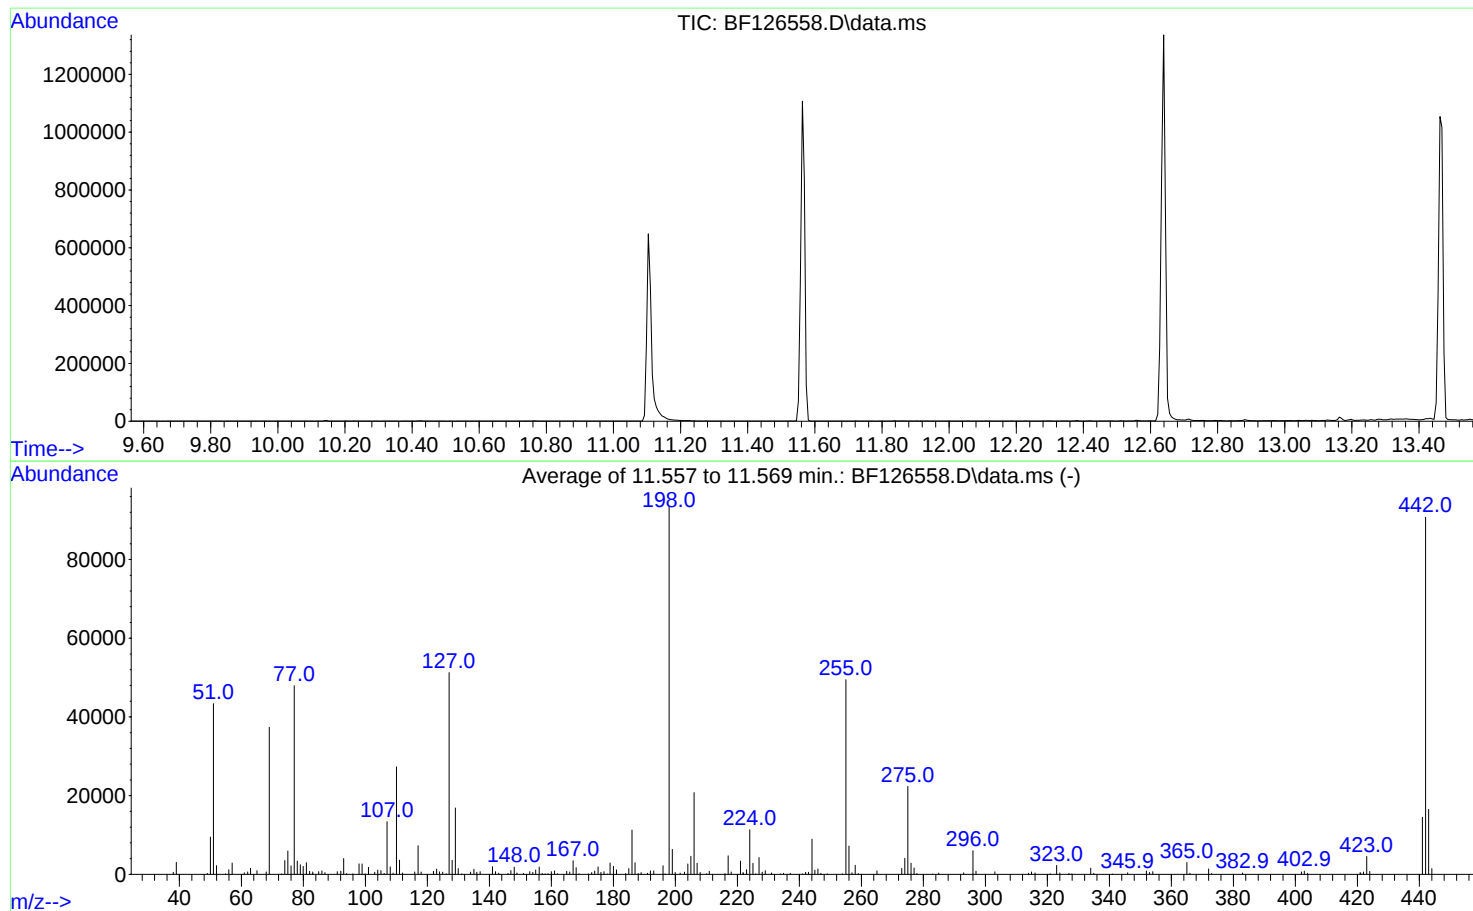




AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	43392	PASS
68	69	0.00	2	1.6	599	PASS
69	198	0.00	100	40.0	37355	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.8	51253	PASS
197	198	0.00	2	0.1	128	PASS
198	198	100	100	100.0	93472	PASS
199	198	5	9	6.8	6342	PASS
275	198	10	60	23.9	22357	PASS
365	198	1	100	3.2	3025	PASS
441	198	0.01	100	15.5	14527	PASS
442	442	50	100	100.0	90736	PASS
443	442	15	24	18.2	16513	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011022\
Data File : BF126558.D
Acq On : 10 Jan 2022 11:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 10 14:58:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 10 14:50:31 2022
Response via : Initial Calibration

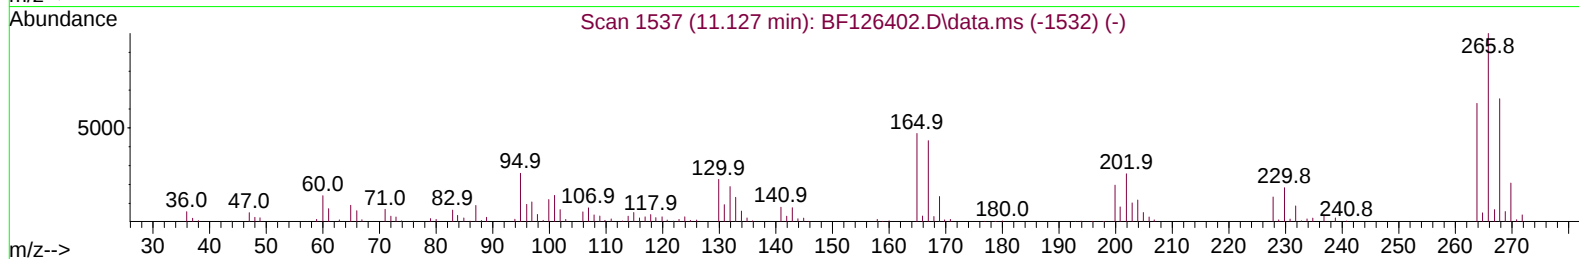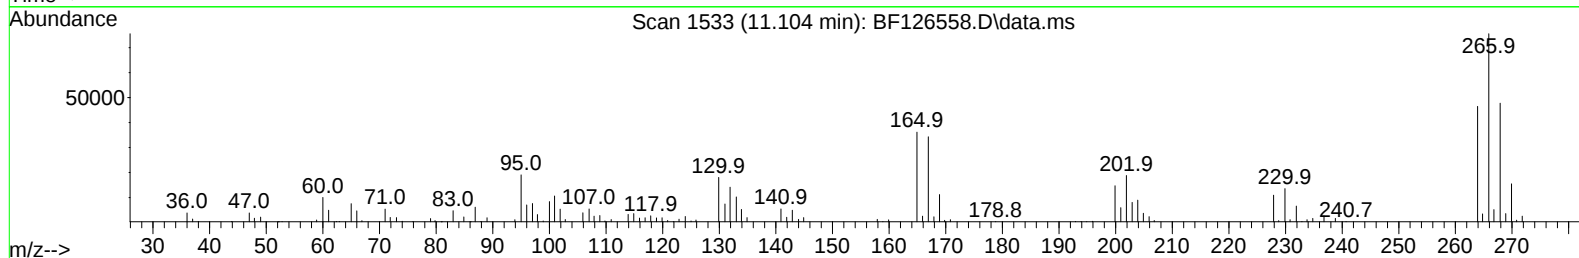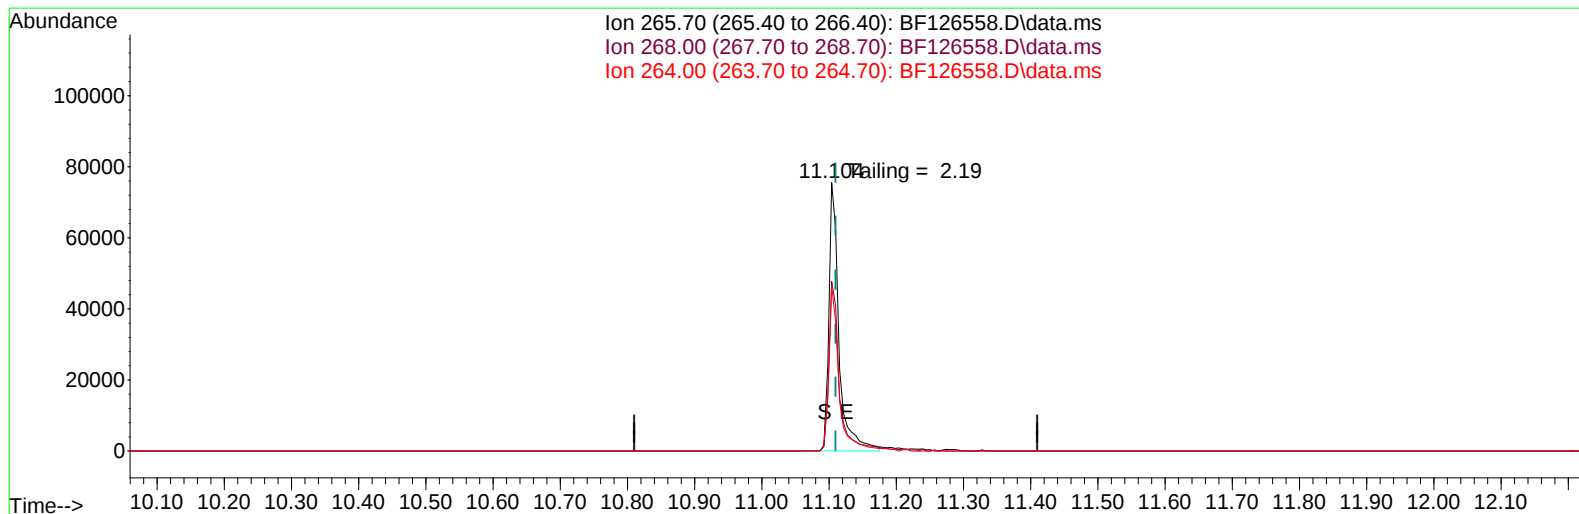

TIC: BF126558.D\data.ms

(70) Pentachlorophenol (C)

11.104min (-0.006) 60587.49 ng




response 81480

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	63.26
264.00	63.00	61.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011022\
Data File : BF126558.D
Acq On : 10 Jan 2022 11:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 10 14:58:21 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 10 14:50:31 2022
Response via : Initial Calibration

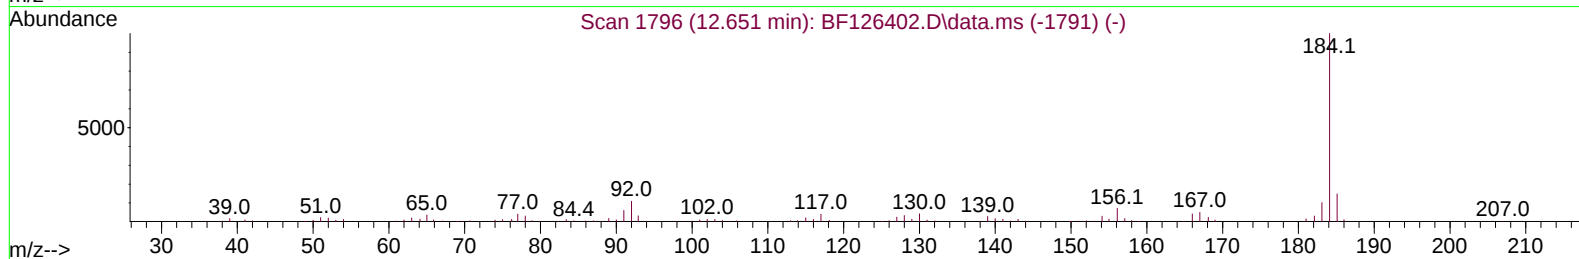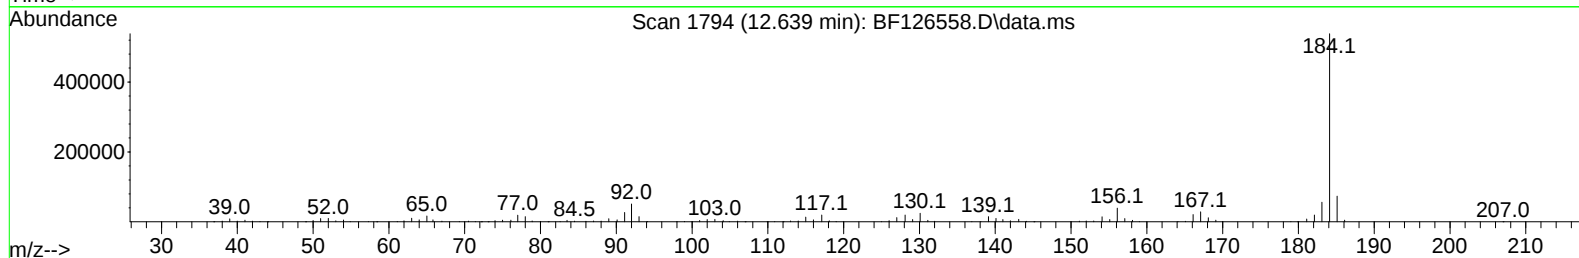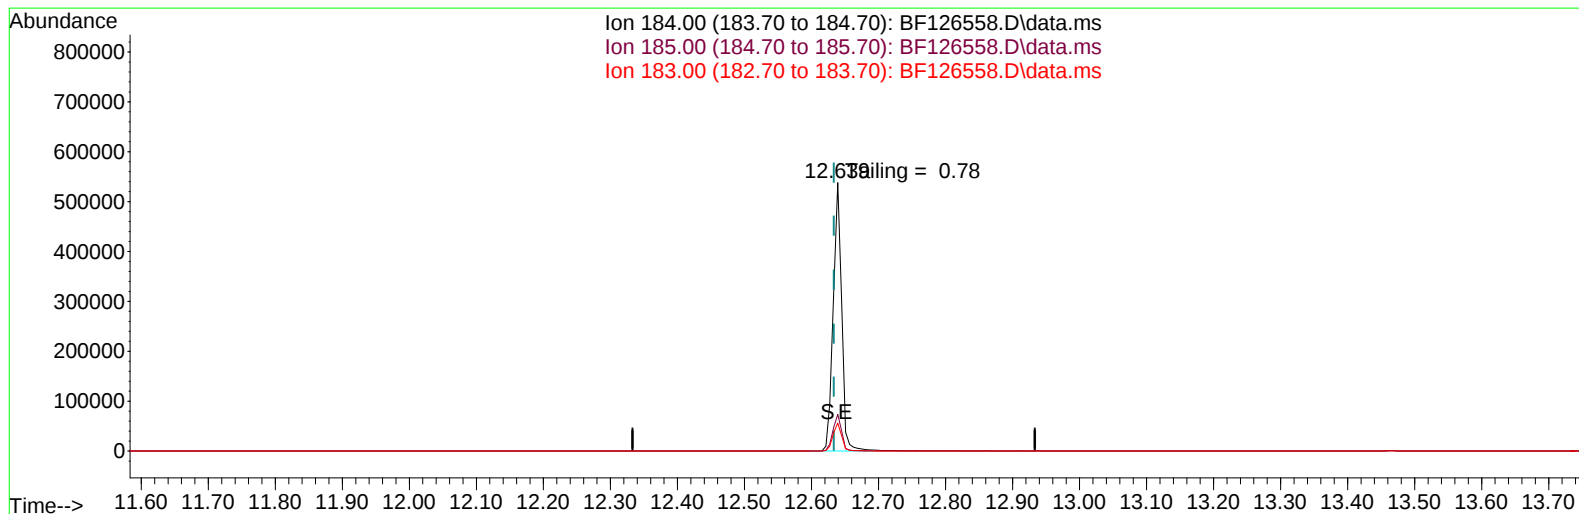

TIC: BF126558.D\data.ms

(77) Benzidine

12.639min (+ 0.006) 0.00 ng

response 476719

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.65
183.00	10.20	10.48
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/10/2022	BNA_F	<u>BF126558.D</u>
Compound Name	Response	Retention Time
DDT	195416	13.46
DDD	2489	13.16
DDE	0	12.97
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2489	197905	1.26

Instrument :
BNA_F
ClientSampleId :
DFTPP