
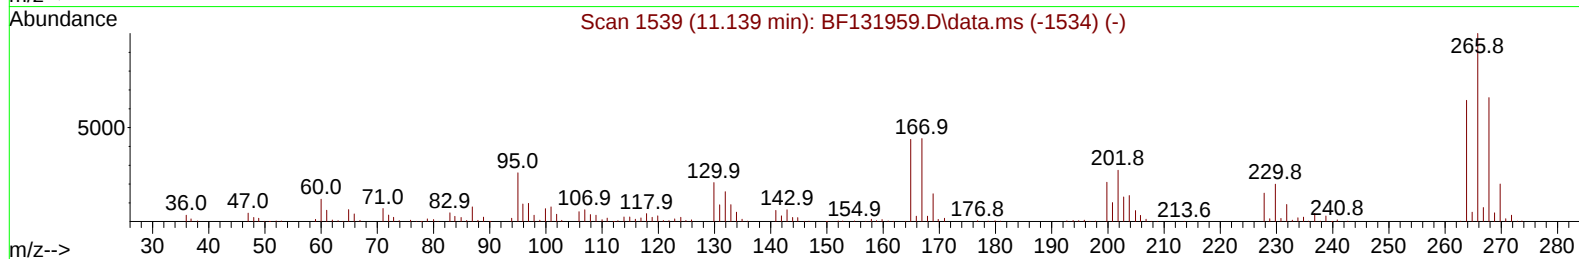
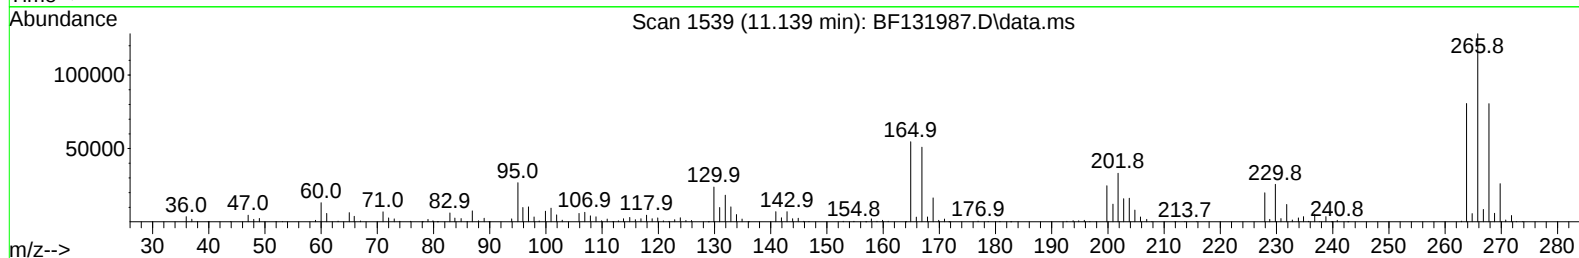


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011023\
 Data File : BF131987.D
 Acq On : 10 Jan 2023 09:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 04:29:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 10 00:32:25 2023
 Response via : Initial Calibration

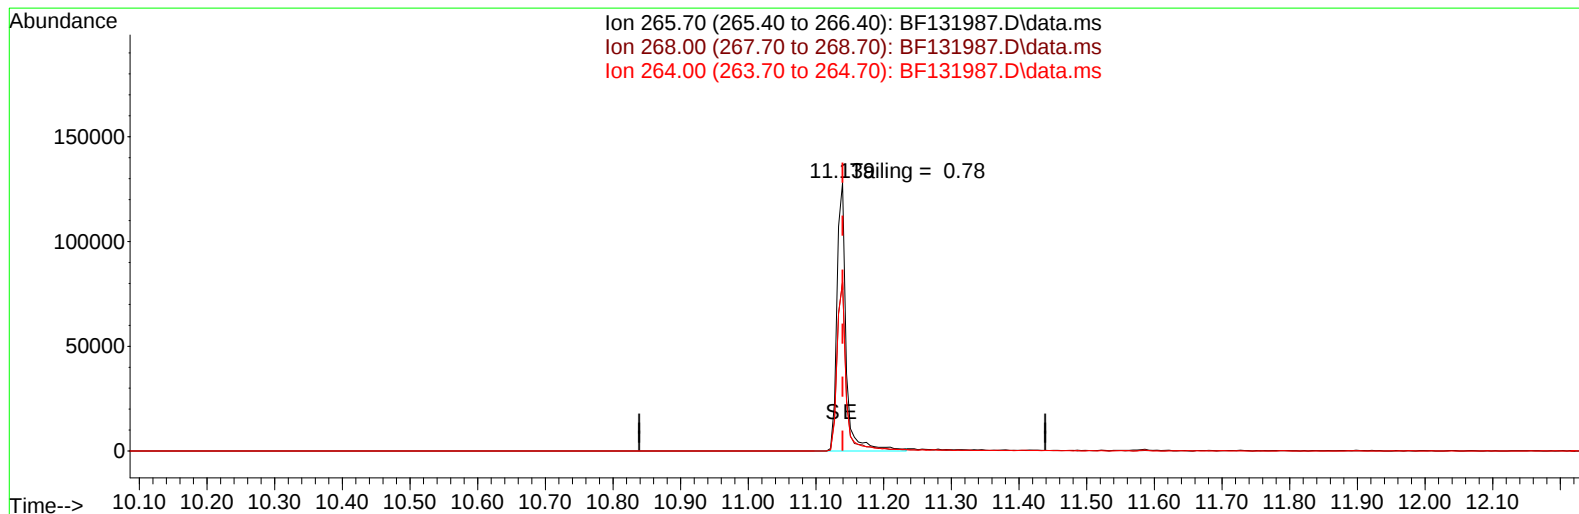

TIC: BF131987.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.000) 23087.19 ng

response 120430

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	62.83
264.00	64.50	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011023\
Data File : BF131987.D
Acq On : 10 Jan 2023 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 04:29:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 00:32:25 2023
Response via : Initial Calibration

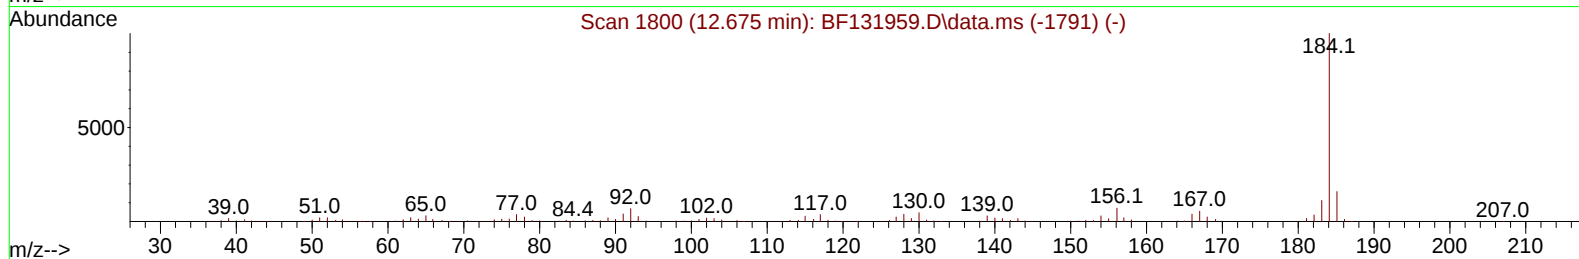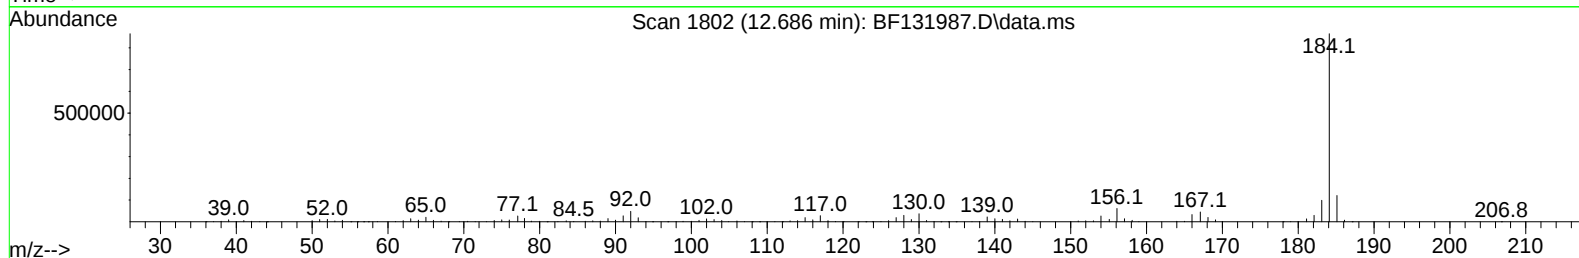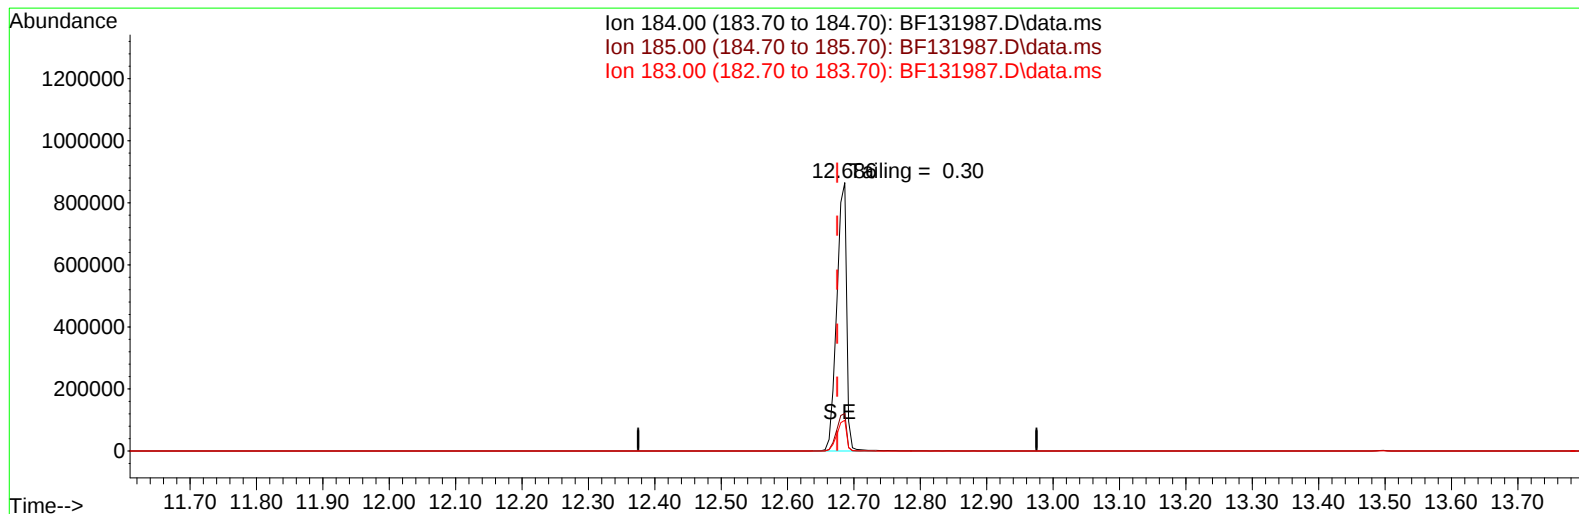

TIC: BF131987.D\data.ms

(77) Benzidine

12.686min (+ 0.011) 0.00 ng

response 891082

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	13.94
183.00	11.20	11.45
0.00	0.00	0.00