


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011023\
Data File : BF131987.D
Acq On : 10 Jan 2023 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 10 00:32:25 2023

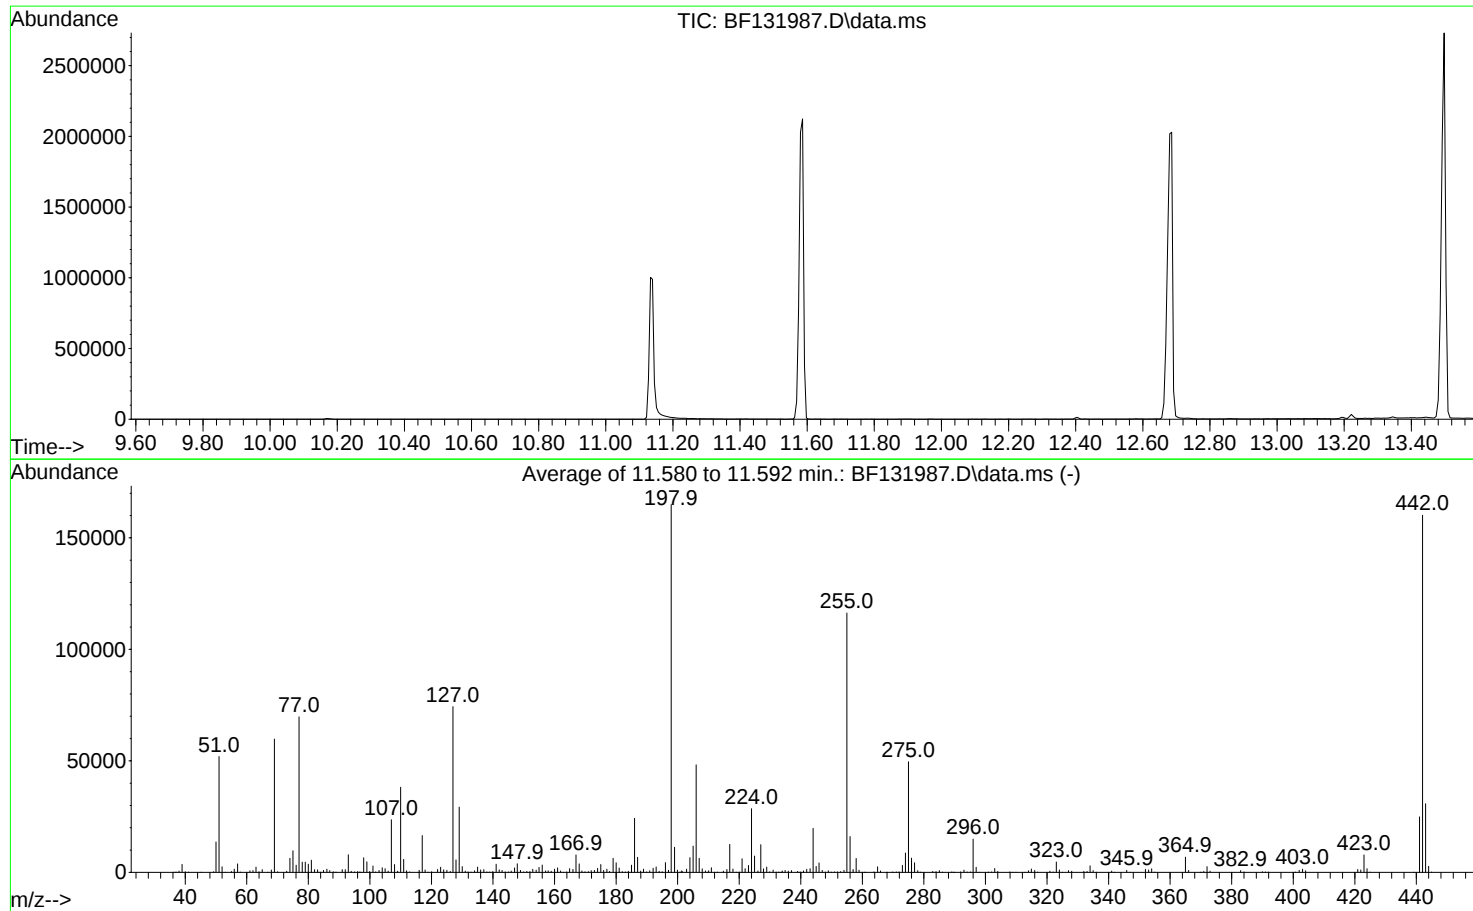




AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.5	51924	PASS
68	69	0.00	2	1.9	1109	PASS
69	198	0.00	100	36.2	59796	PASS
70	69	0.00	2	0.5	287	PASS
127	198	10	80	45.1	74353	PASS
197	198	0.00	2	0.6	962	PASS
198	198	100	100	100.0	164957	PASS
199	198	5	9	6.8	11247	PASS
275	198	10	60	30.0	49567	PASS
365	198	1	100	4.1	6805	PASS
441	198	0.01	100	15.1	24893	PASS
442	442	50	100	100.0	160117	PASS
443	442	15	24	19.2	30795	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011023\
 Data File : BF131987.D
 Acq On : 10 Jan 2023 09:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 11 04:29:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 10 00:32:25 2023
 Response via : Initial Calibration

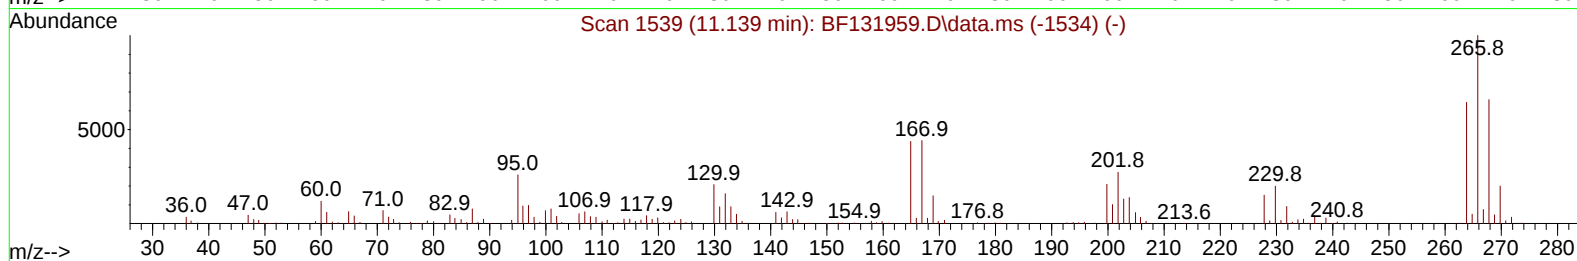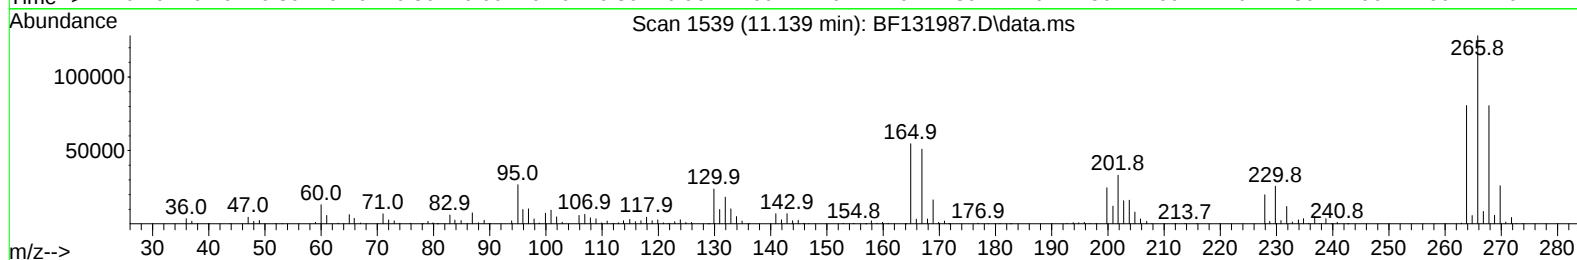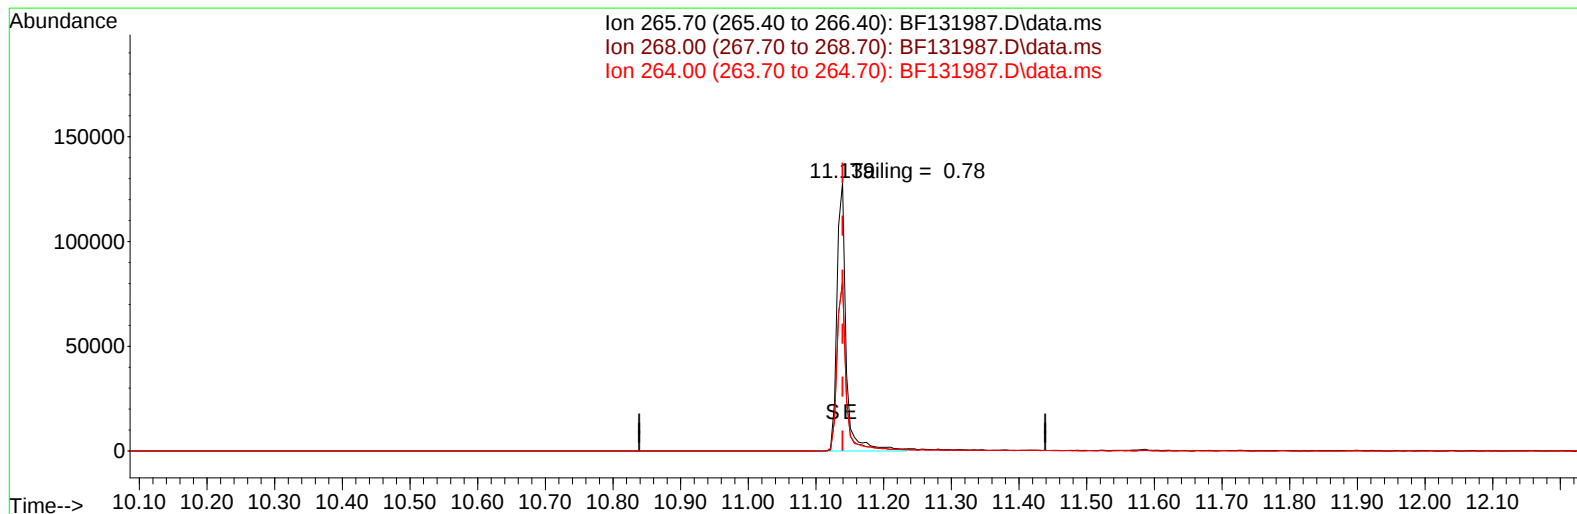

TIC: BF131987.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 23087.19 ng




response 120430

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	62.83
264.00	64.50	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011023\
Data File : BF131987.D
Acq On : 10 Jan 2023 09:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 11 04:29:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 00:32:25 2023
Response via : Initial Calibration

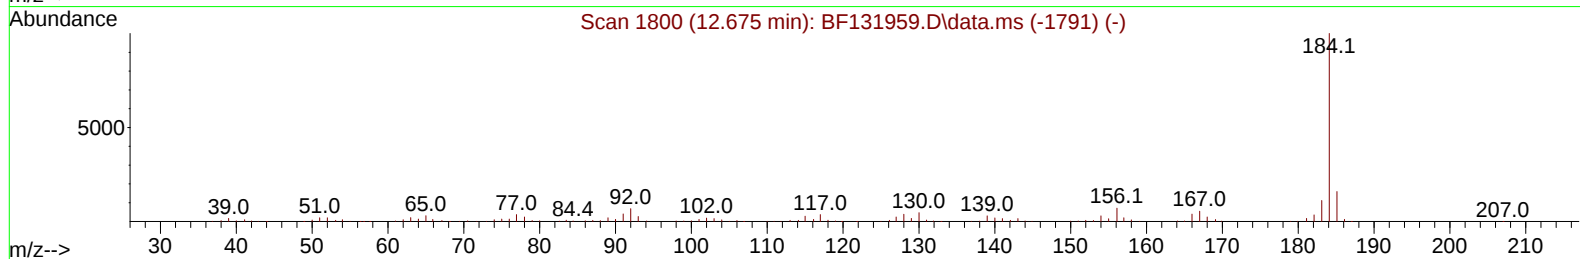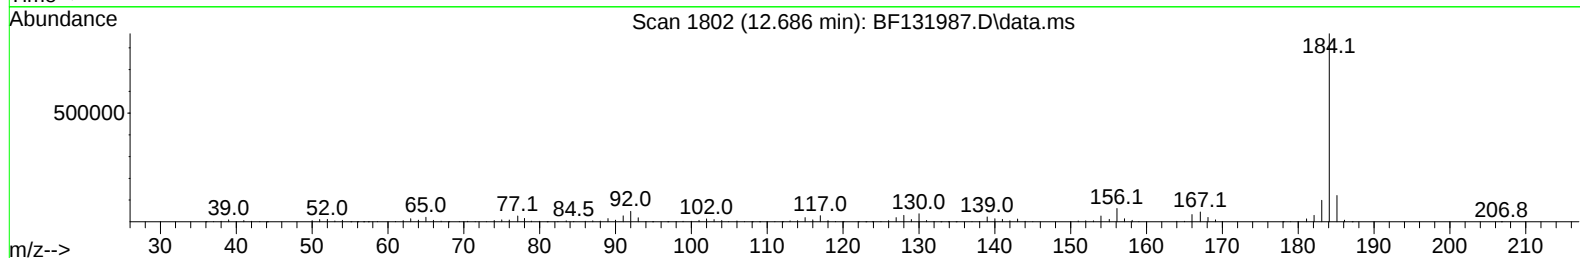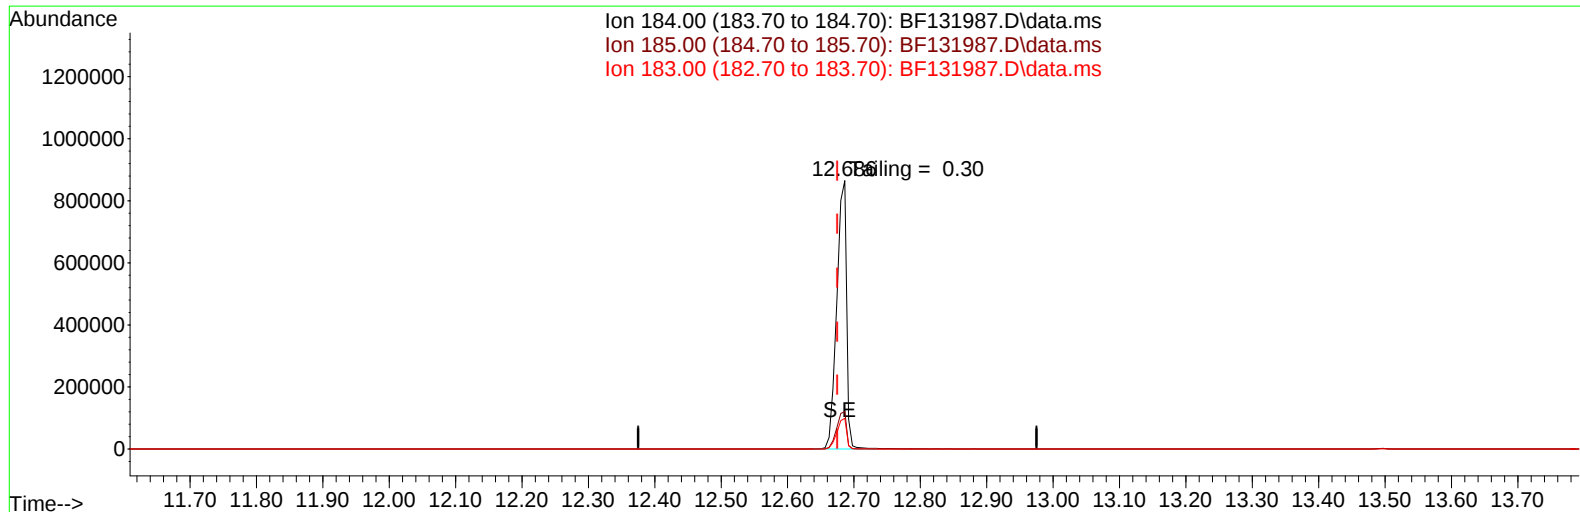

TIC: BF131987.D\data.ms

(77) Benzidine

12.686min (+ 0.011) 0.00 ng

response 891082

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	13.94
183.00	11.20	11.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/10/2023	BNA_F	<u>BF131987.D</u>
Compound Name	Response	Retention Time
DDT	454971	13.498
DDD	6285	13.221
DDE	884	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7169	462140	1.55

Instrument :
BNA_F
ClientSampleId :
DFTPP