
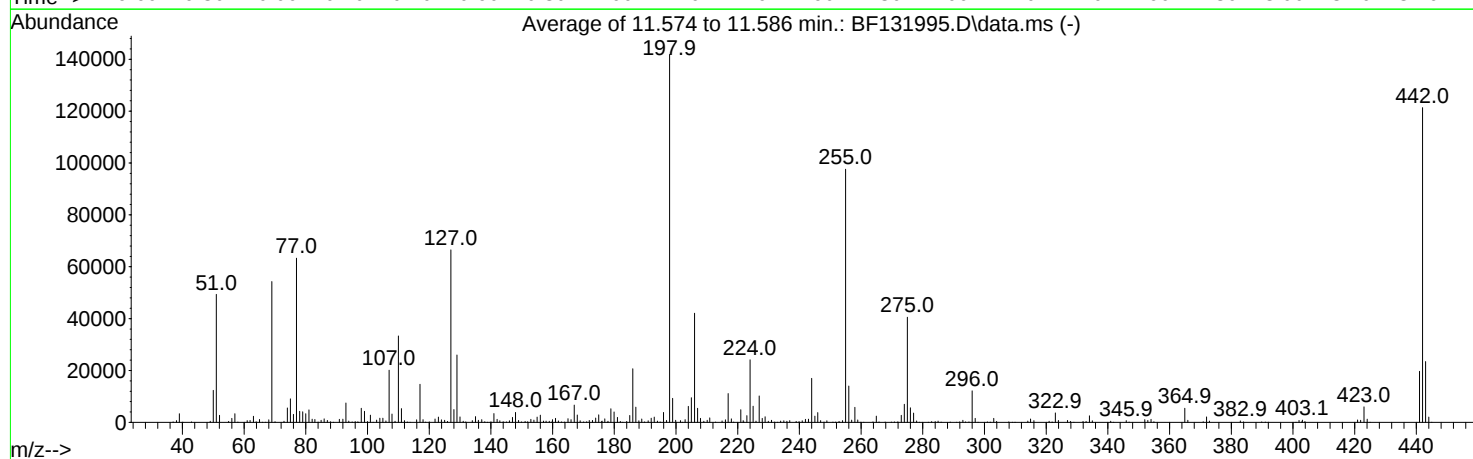


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011023\
 Data File : BF131995.D
 Acq On : 10 Jan 2023 14:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 10 00:32:25 2023

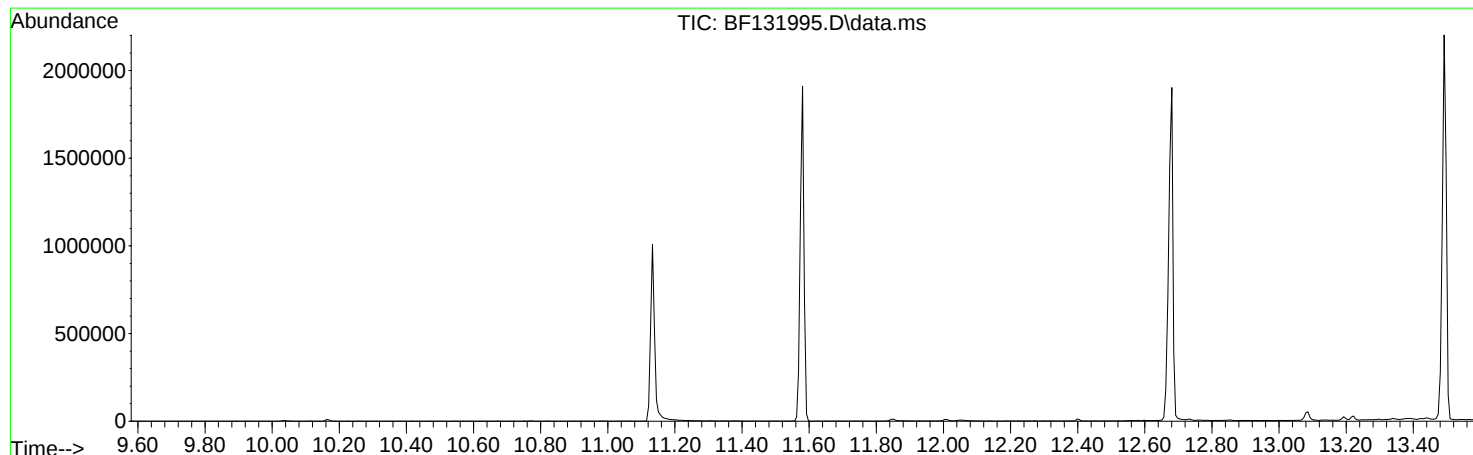




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	49349	PASS
68	69	0.00	2	1.8	989	PASS
69	198	0.00	100	38.3	54302	PASS
70	69	0.00	2	0.5	267	PASS
127	198	10	80	46.9	66491	PASS
197	198	0.00	2	0.5	736	PASS
198	198	100	100	100.0	141837	PASS
199	198	5	9	6.5	9284	PASS
275	198	10	60	28.6	40512	PASS
365	198	1	100	3.8	5453	PASS
441	198	0.01	100	13.9	19696	PASS
442	442	50	100	100.0	121373	PASS
443	442	15	24	19.3	23435	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011023\  
Data File : BF131995.D  
Acq On    : 10 Jan 2023  14:33  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 11 04:31:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 00:32:25 2023
Response via : Initial Calibration

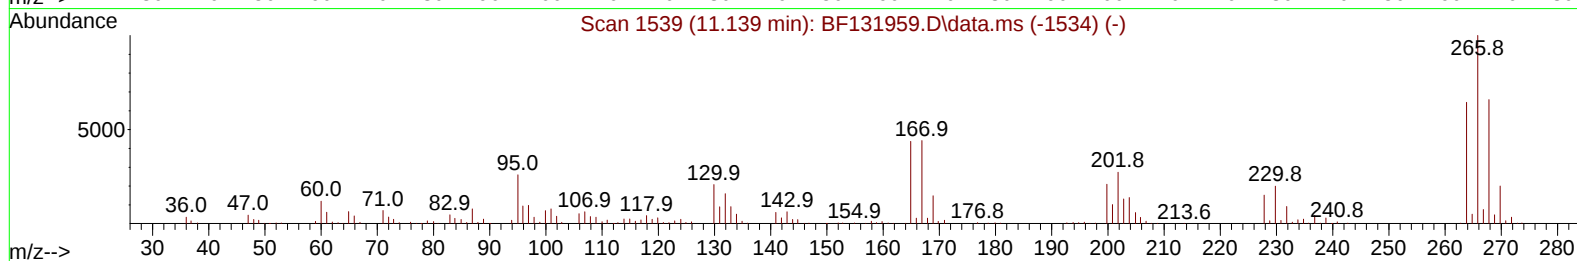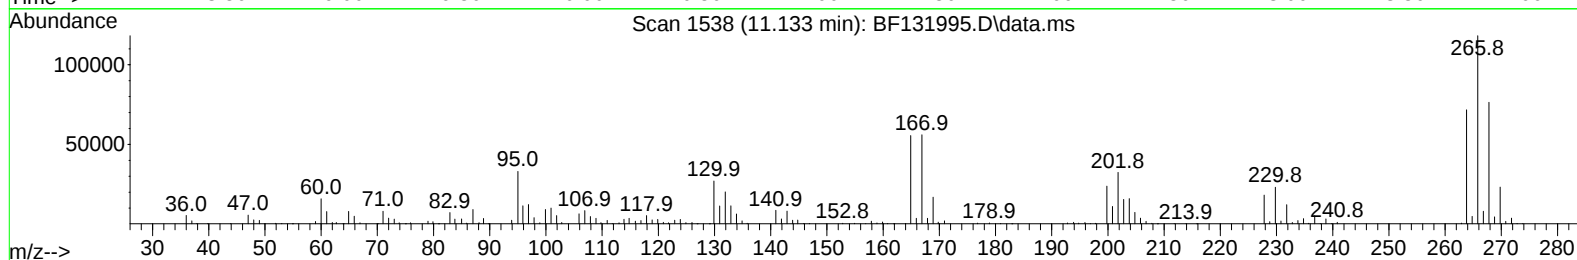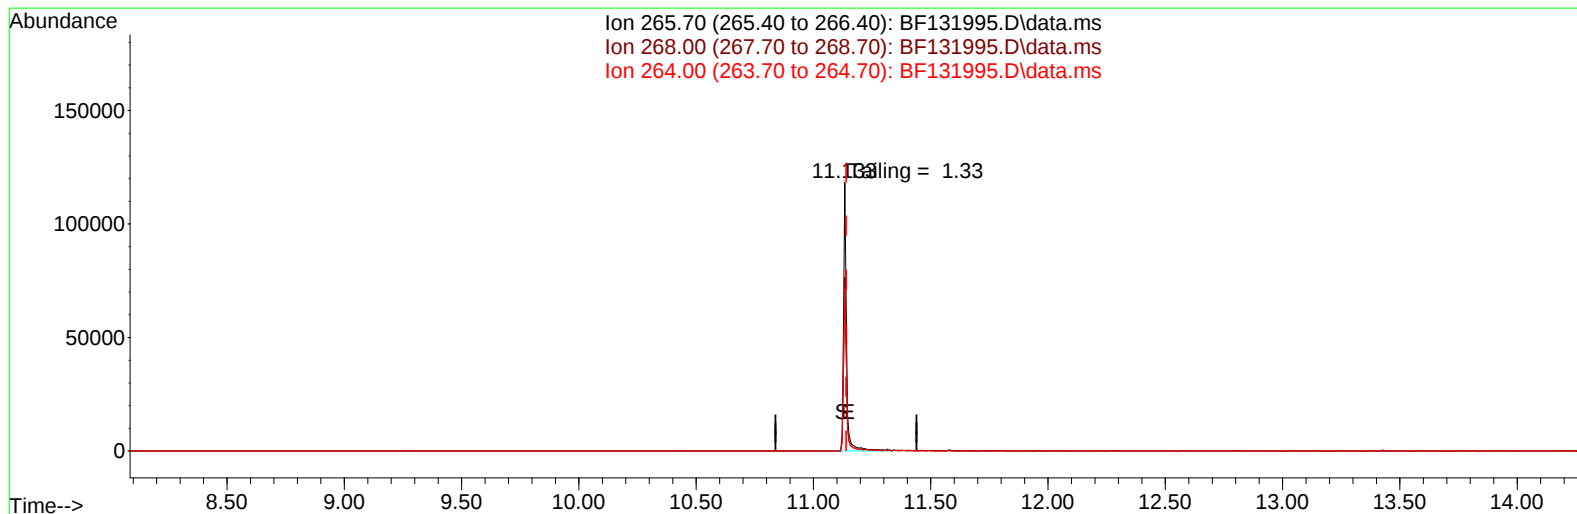

TIC: BF131995.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.006) 20586.78 ng




response **103859**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.90	64.63
264.00	64.50	60.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011023\
 Data File : BF131995.D
 Acq On : 10 Jan 2023 14:33
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 11 04:31:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF010923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 10 00:32:25 2023
 Response via : Initial Calibration

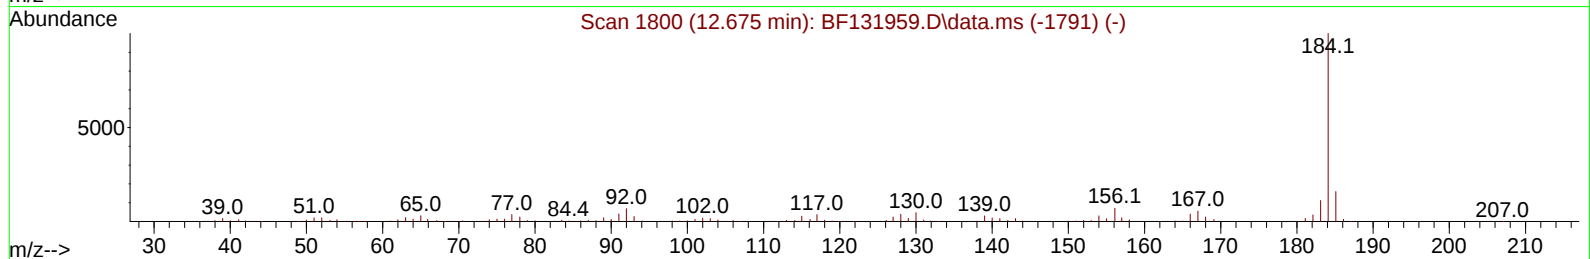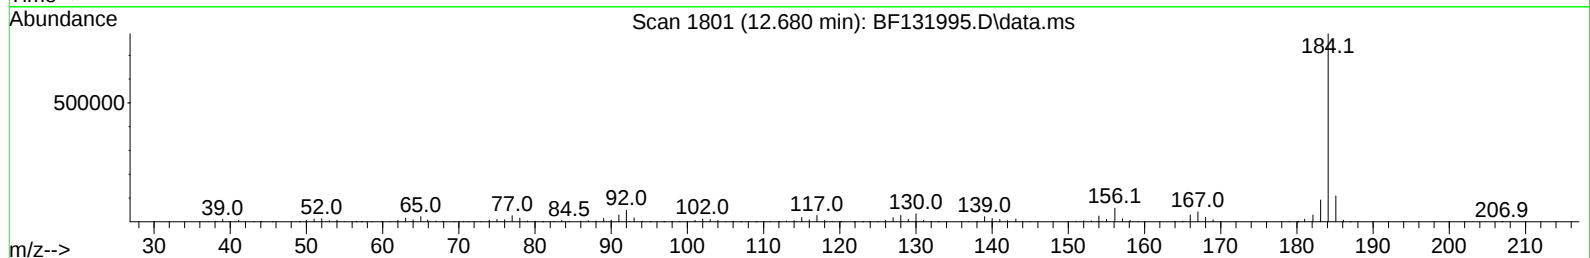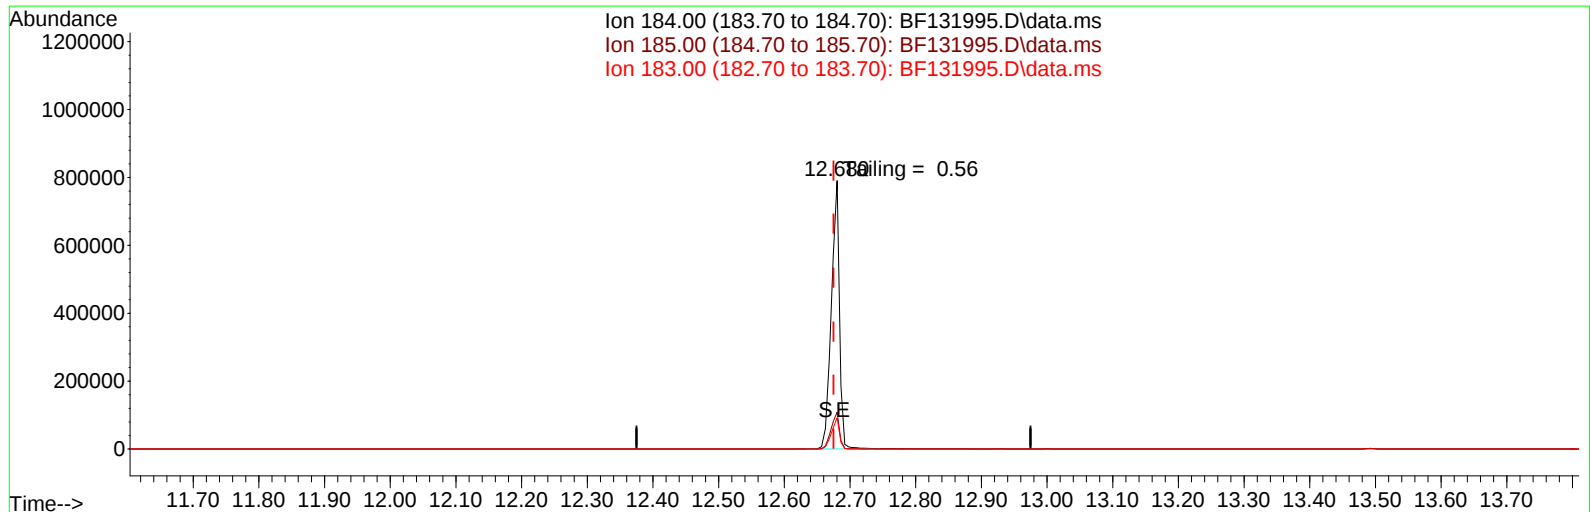

TIC: BF131995.D\data.ms

(77) Benzidine

12.680min (+ 0.005) 0.00 ng

response 679404

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	13.72
183.00	11.20	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/10/2023	BNA_F	<u>BF131995.D</u>
Compound Name	Response	Retention Time
DDT	358503	13.492
DDD	7117	13.221
DDE	573	12.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7690	366193	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP