
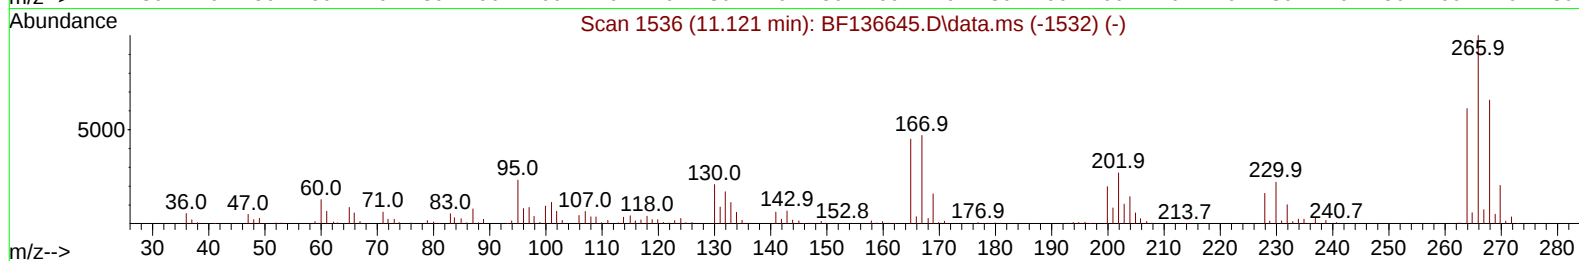
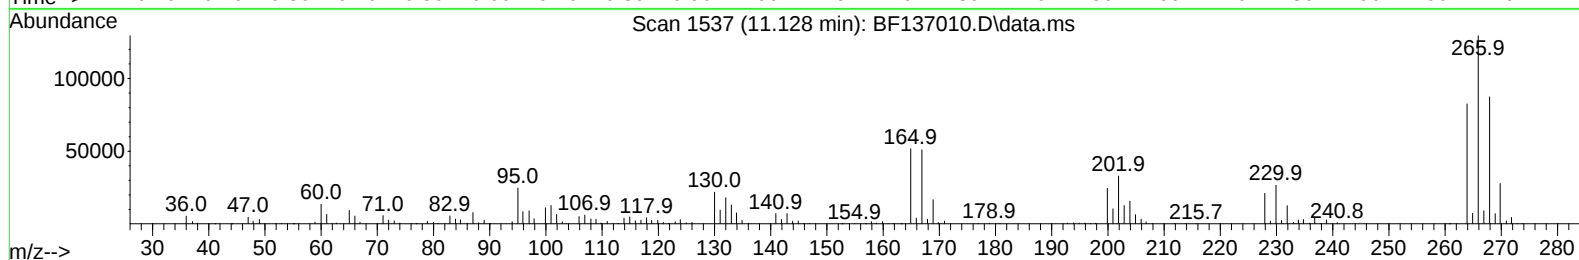


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011024\
 Data File : BF137010.D
 Acq On : 10 Jan 2024 09:53
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 11:17:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 21 01:54:25 2023
 Response via : Initial Calibration

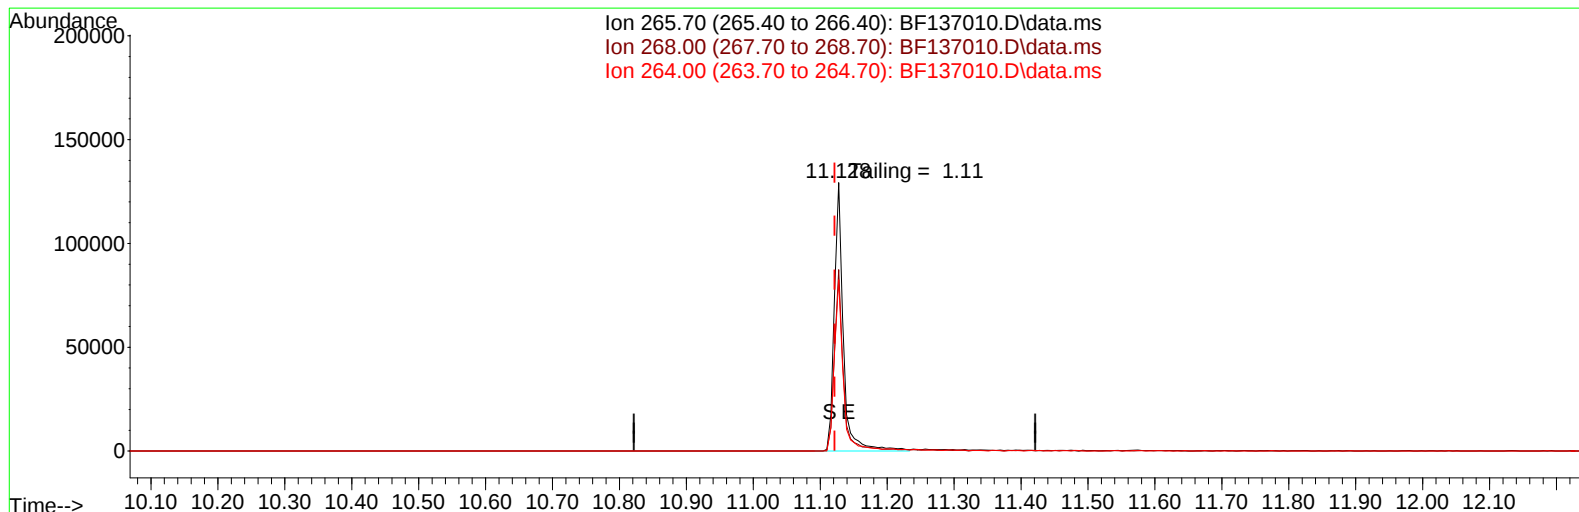




TIC: BF137010.D\data.ms

(70) Pentachlorophenol (C)**11.128min (+ 0.006) 394522.18 ng****response 122899**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.70	67.57
264.00	61.20	63.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011024\
Data File : BF137010.D
Acq On : 10 Jan 2024 09:53
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 11:17:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 21 01:54:25 2023
Response via : Initial Calibration

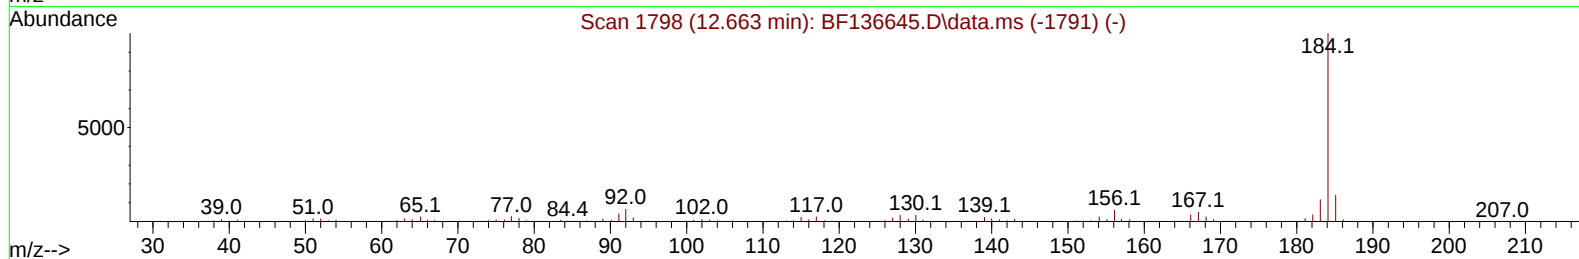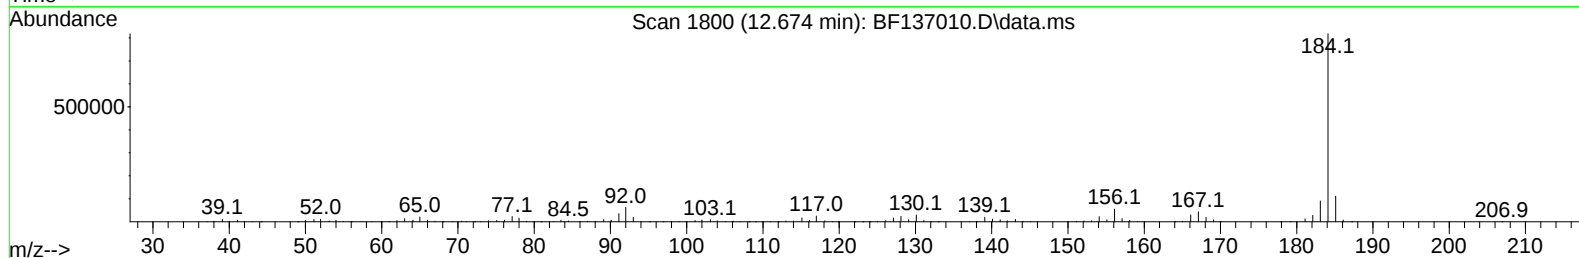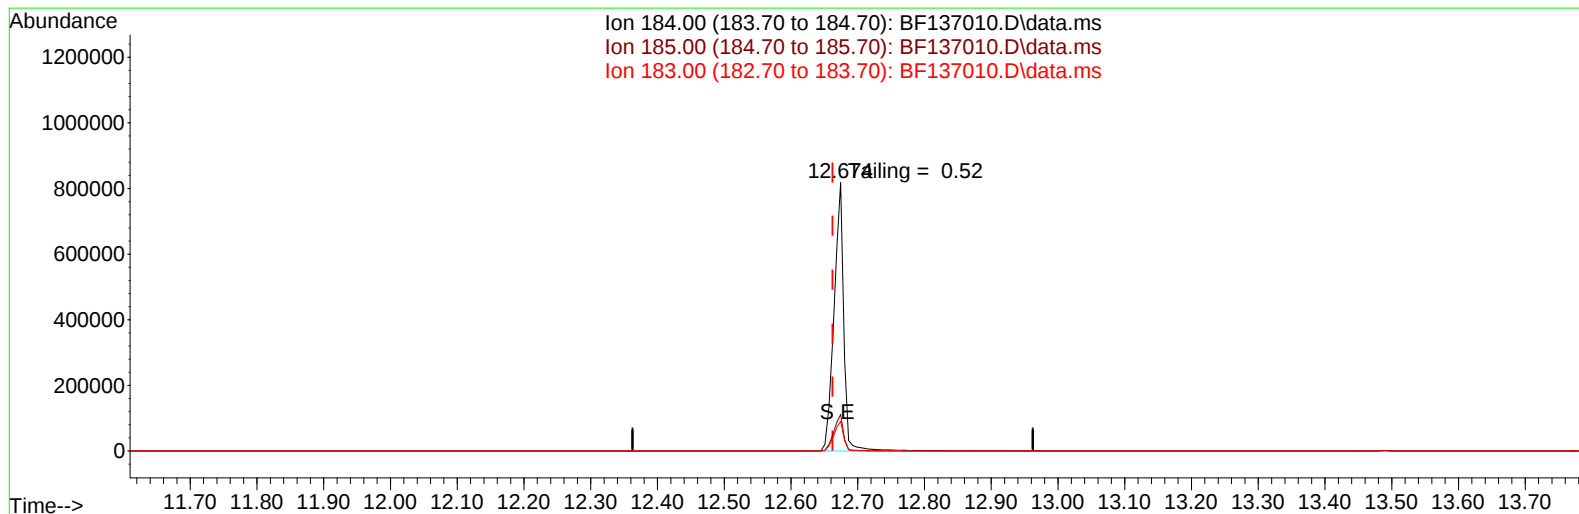

TIC: BF137010.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 412472.37 ng

response 827019

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.66
183.00	11.60	11.10
0.00	0.00	0.00