

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011024\
 Data File : BF137031.D
 Acq On : 10 Jan 2024 21:05
 Operator : CG\JU
 Sample : P1069-01 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EO-01-010824

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.004	492	496	503	rVB2	6727	8802	2.68%	0.346%
2	5.434	566	569	587	rBV	114439	134169	40.79%	5.276%
3	6.440	737	740	757	rBV	92552	128464	39.05%	5.052%
4	6.787	795	799	806	rVB	289984	235036	71.45%	9.243%
5	7.345	891	894	903	rBV	82032	76704	23.32%	3.016%
6	8.063	1012	1016	1023	rBV	319277	260506	79.19%	10.245%
7	9.139	1195	1199	1208	rBV	166371	160570	48.81%	6.315%
8	9.516	1260	1263	1269	rVB5	7297	9196	2.80%	0.362%
9	9.822	1311	1315	1323	rVB	316350	279491	84.96%	10.991%
10	10.616	1447	1450	1457	rBV	93398	88848	27.01%	3.494%
11	11.316	1565	1569	1579	rBV	371159	325346	98.90%	12.795%
12	11.845	1657	1659	1666	rBV7	9038	13921	4.23%	0.547%
13	12.539	1774	1777	1779	rBV3	8124	8686	2.64%	0.342%
14	12.763	1813	1815	1819	rBV2	12222	16580	5.04%	0.652%
15	12.863	1828	1832	1834	rBV5	8286	11781	3.58%	0.463%
16	12.904	1836	1839	1843	rBV	248136	223799	68.03%	8.801%
17	13.974	2017	2021	2027	rBV	374125	328952	100.00%	12.936%
18	15.468	2271	2275	2282	rVB	183972	231990	70.52%	9.123%




Sum of corrected areas: 2542841

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011024\
Data File : BF137031.D
Acq On : 10 Jan 2024 21:05
Operator : CG\JU
Sample : P1069-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-010824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

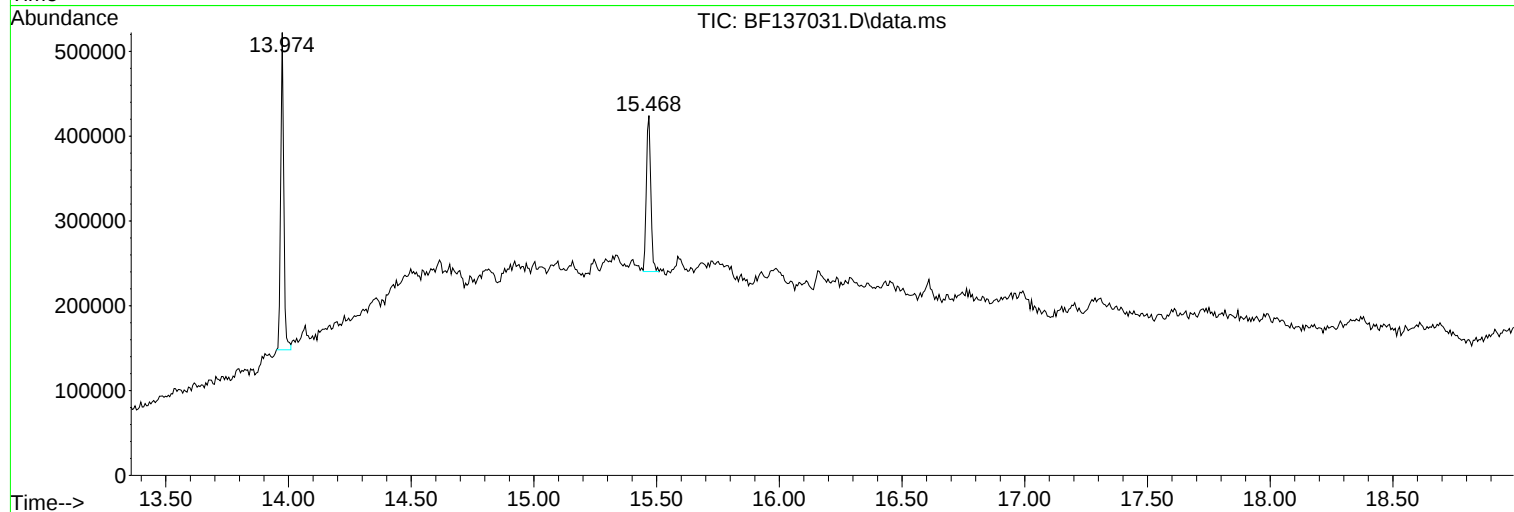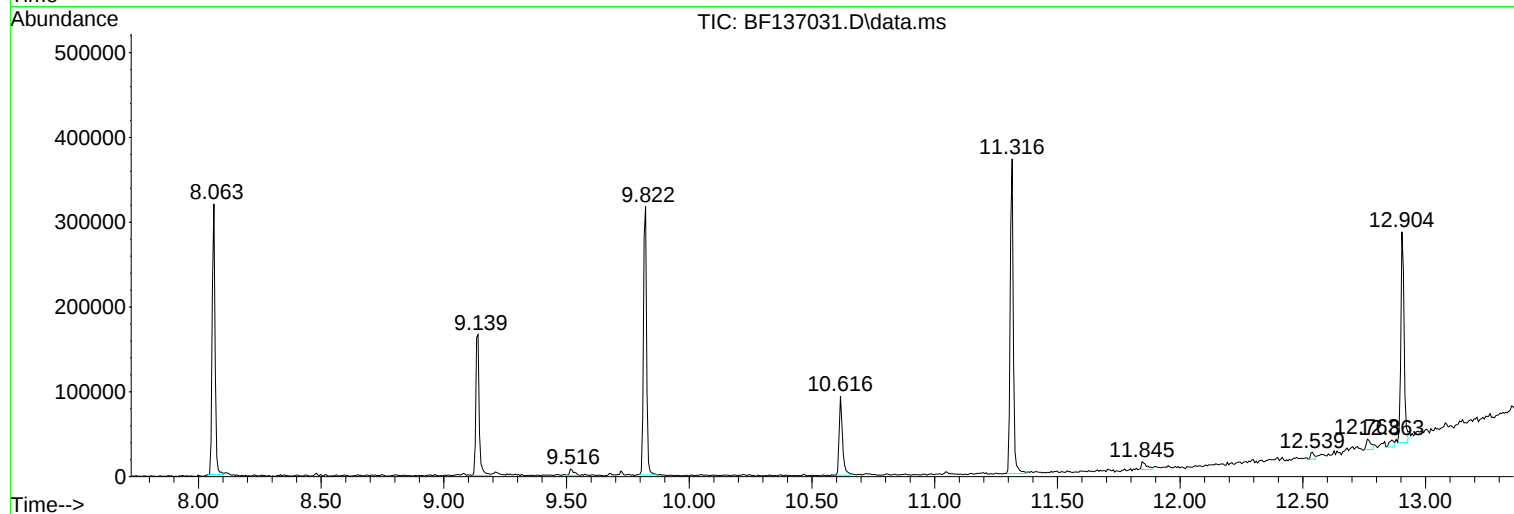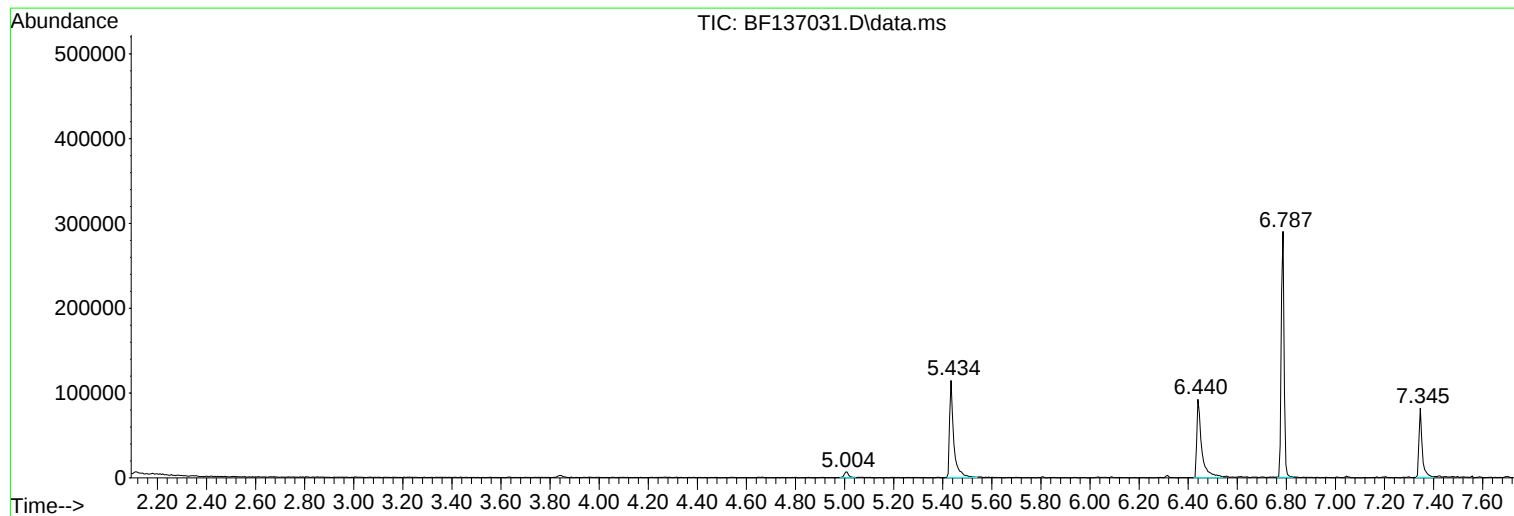

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011024\
Data File : BF137031.D
Acq On : 10 Jan 2024 21:05
Operator : CG\JU
Sample : P1069-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-010824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011024\
Data File : BF137031.D
Acq On : 10 Jan 2024 21:05
Operator : CG\JU
Sample : P1069-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EO-01-010824

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF122023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------