
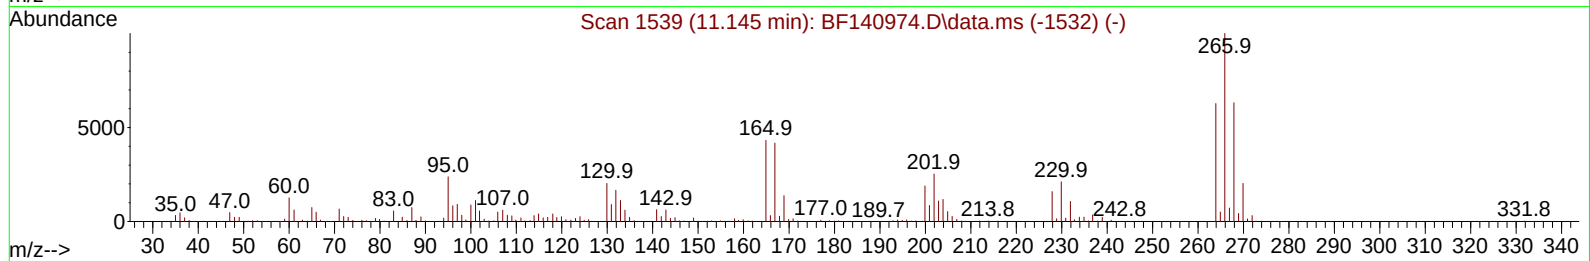
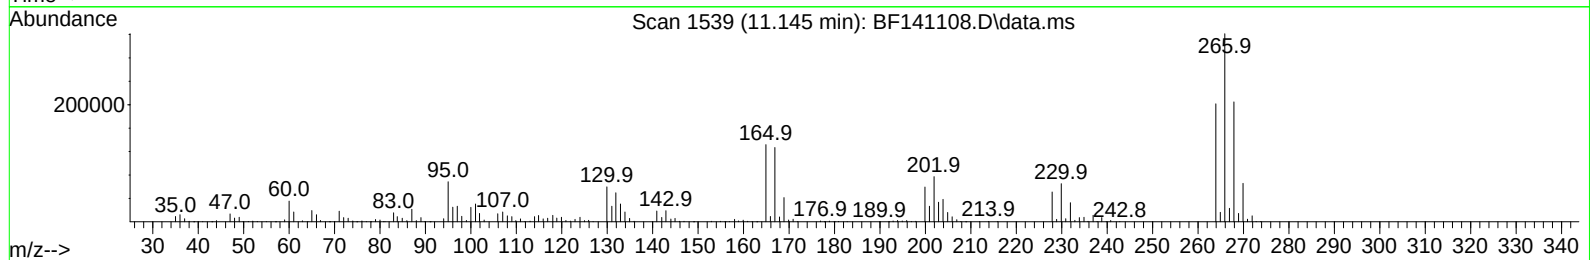


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011025\
Data File : BF141108.D
Acq On : 10 Jan 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 12:08:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 12:07:52 2025
Response via : Initial Calibration

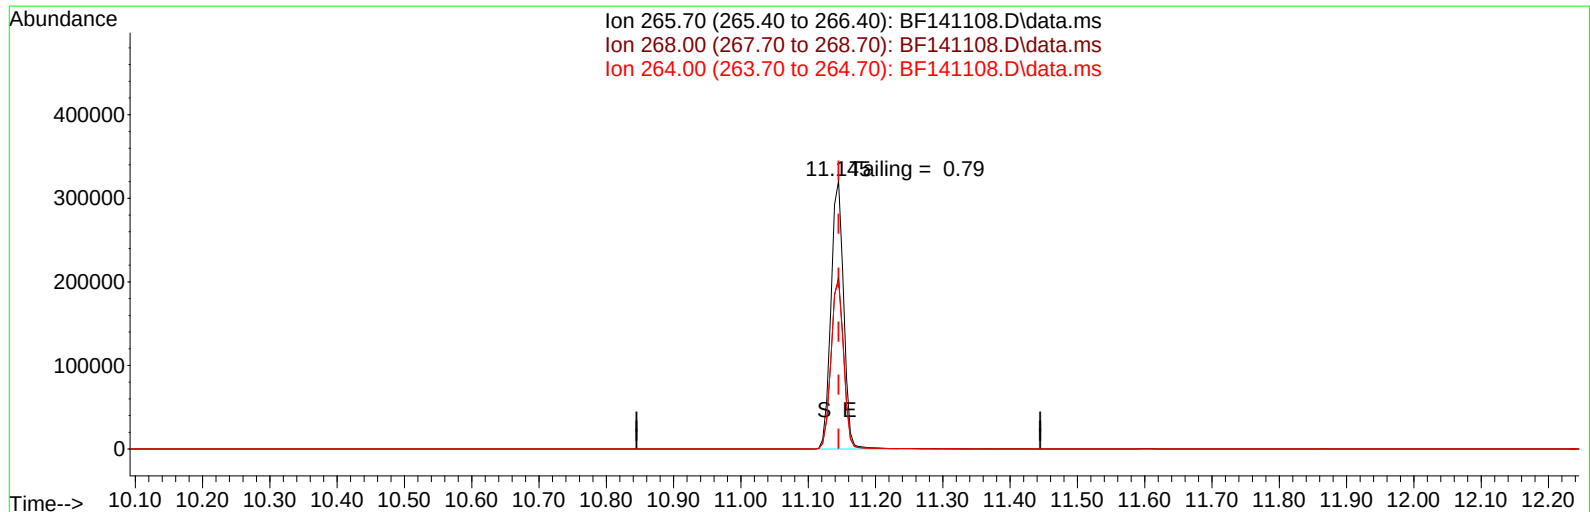

TIC: BF141108.D\data.ms

(70) Pentachlorophenol (C)




11.145min (+ 0.000) 27837.42 ng

response 420211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.79
264.00	62.80	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF011025\
Data File : BF141108.D
Acq On : 10 Jan 2025 11:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 12:08:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 10 12:07:52 2025
Response via : Initial Calibration

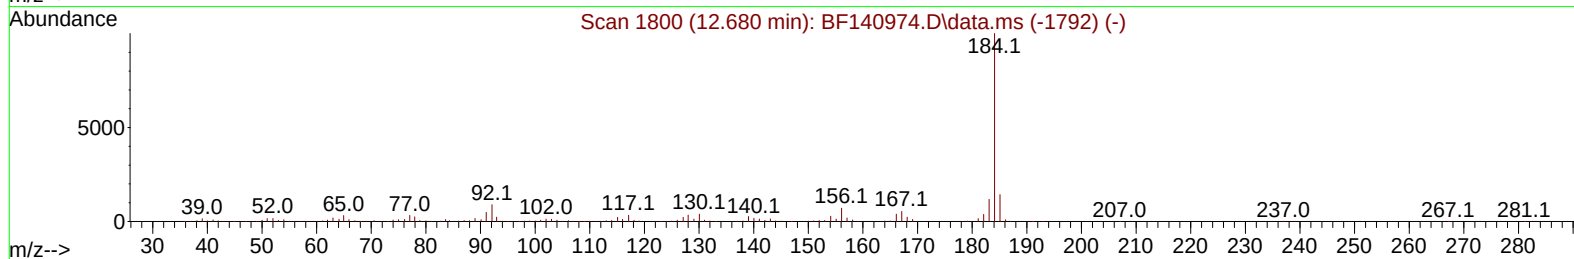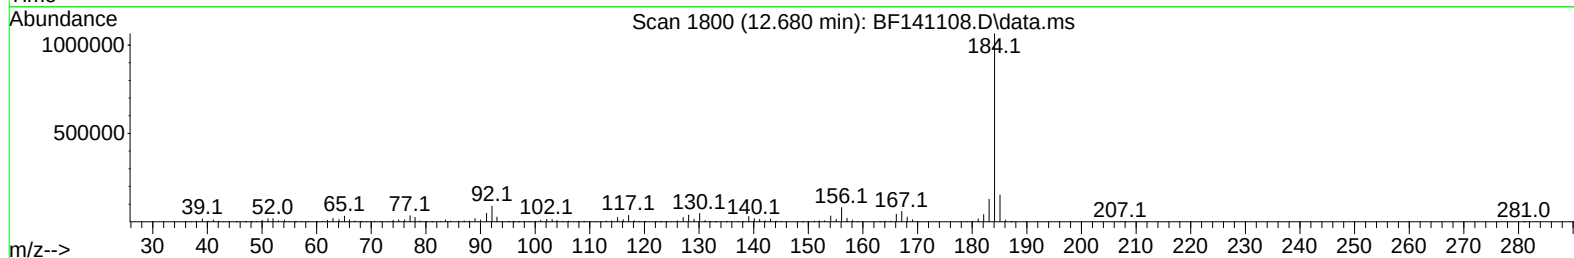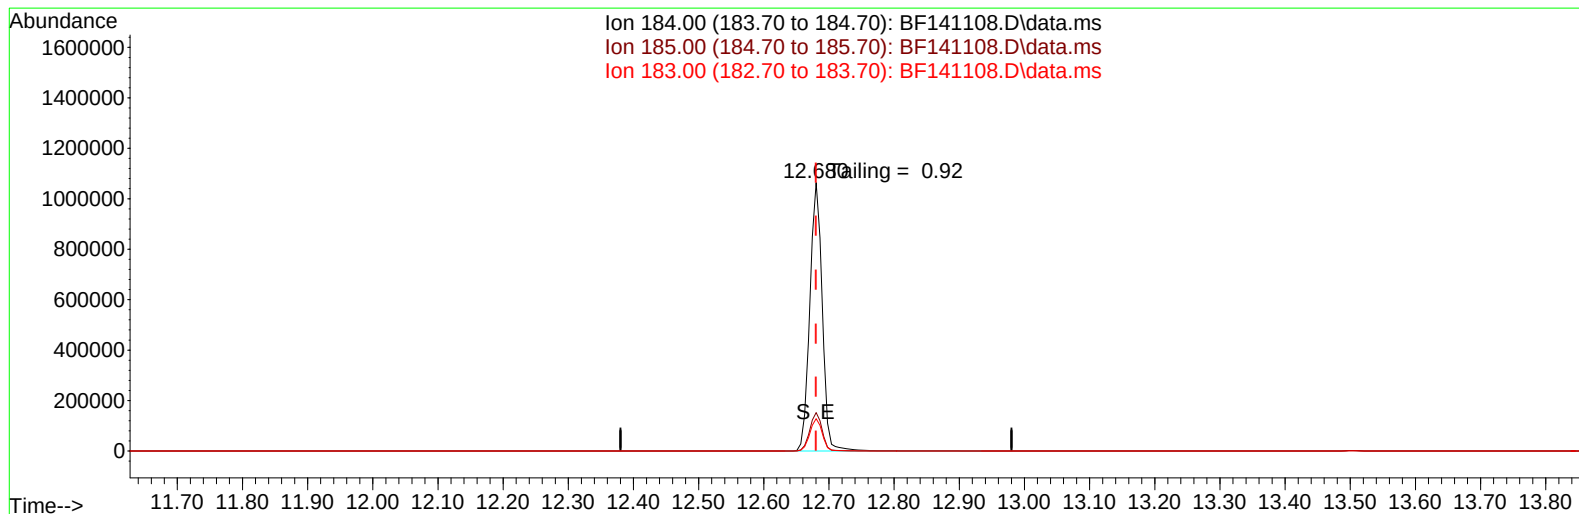

TIC: BF141108.D\data.ms

(77) Benzidine**12.680min (-0.000) 47053.75 ng****response 1415080**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.35
183.00	11.70	12.05
0.00	0.00	0.00