
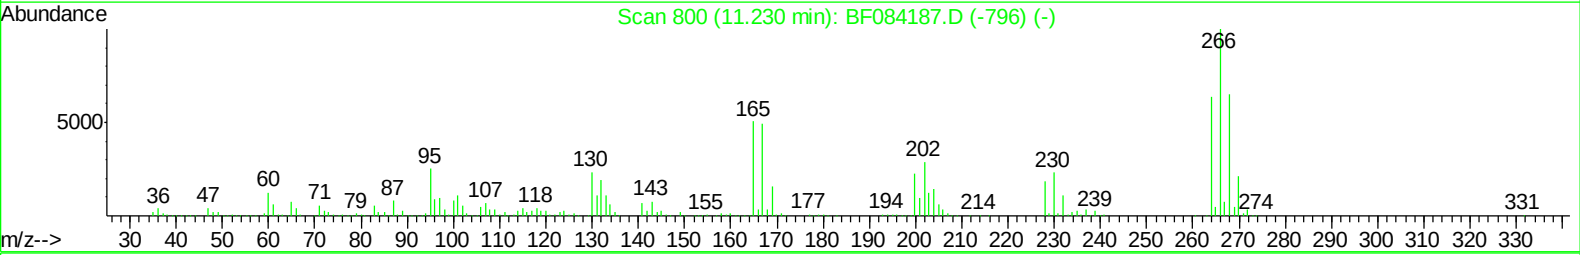
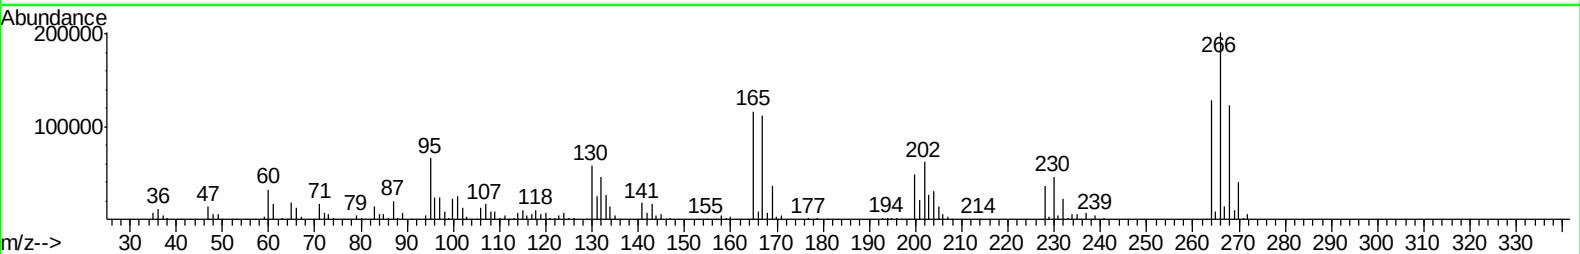





```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\  
Data File : BF084371.D  
Acq On    : 11 Jan 2016    8:55  
Operator  : SJ/UM  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

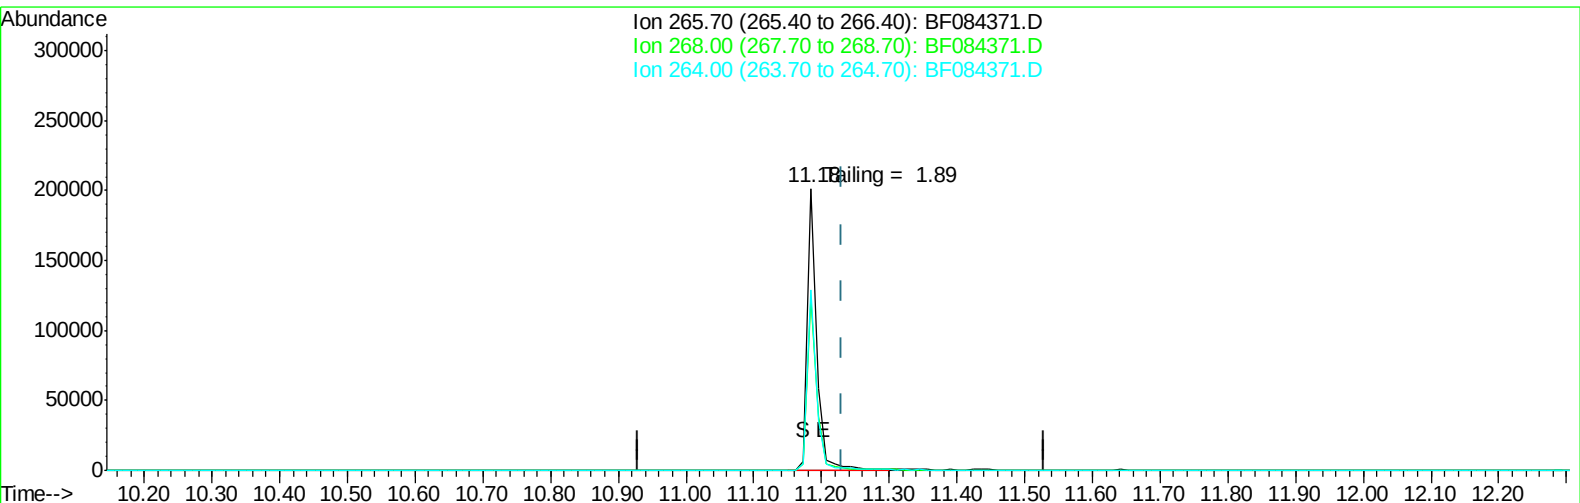

(69) Pentachlorophenol (C)		
11.185min (-0.045) 9531.91ng		
response 199081		
Ion	Exp%	Act%
265.70	100	100
268.00	65.50	60.86
264.00	62.70	64.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
Data File : BF084371.D
Acq On : 11 Jan 2016 8:55
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 07:41:12 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

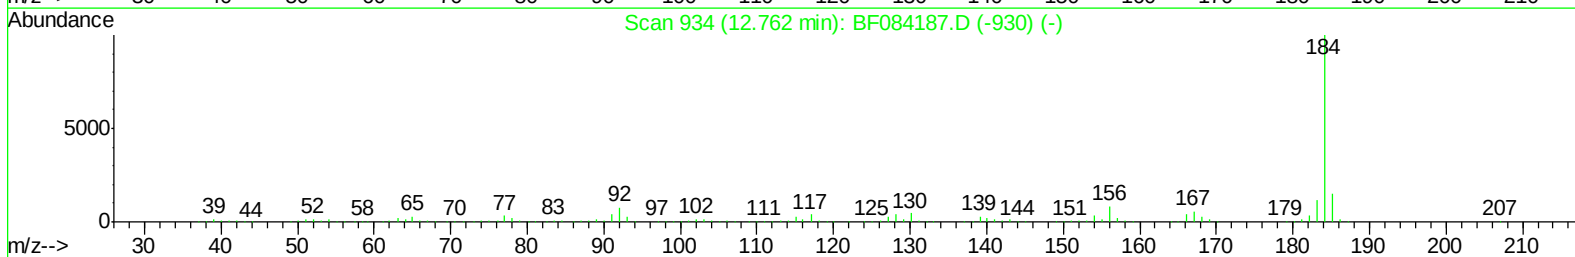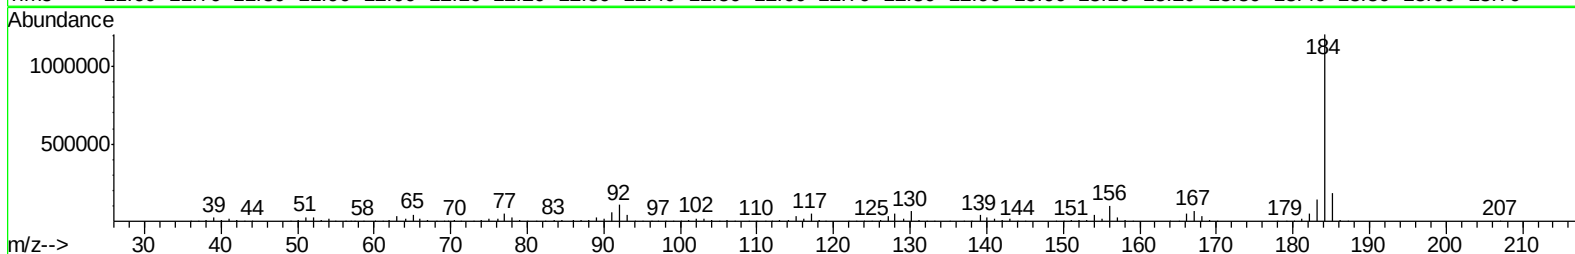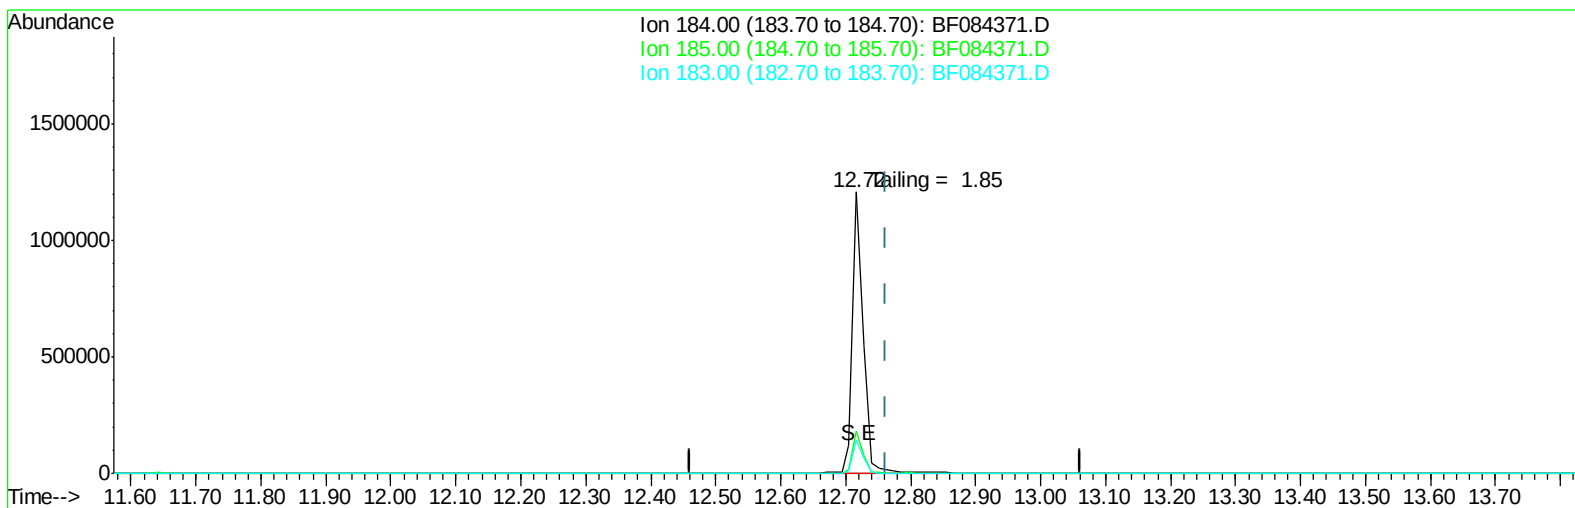

TIC: BF084371.D

(76) Benzidine

12.716min (-0.046) 9577.26ng

response 1374260

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.87
183.00	12.30	11.79
0.00	0.00	0.00