
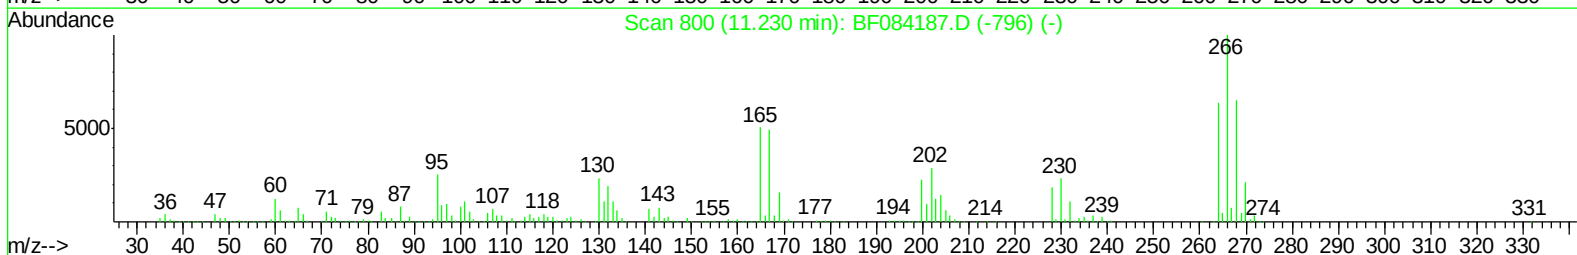
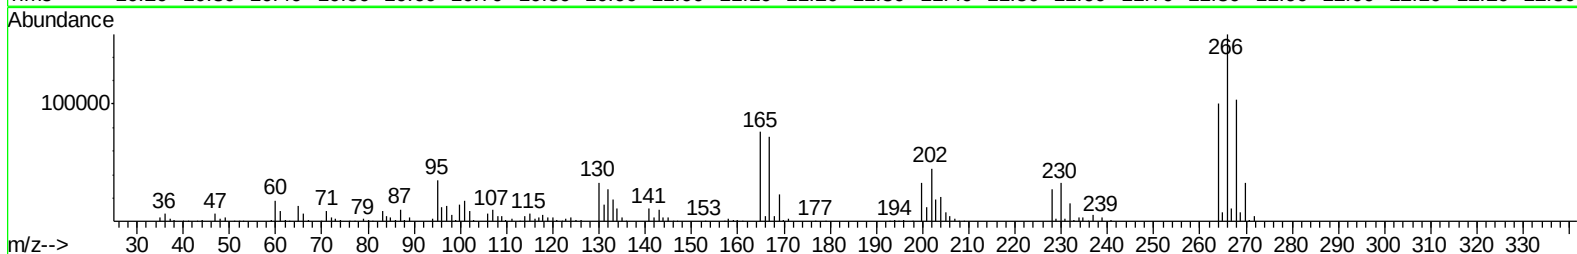


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
Data File : BF084392.D
Acq On : 11 Jan 2016 21:03
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 07:42:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

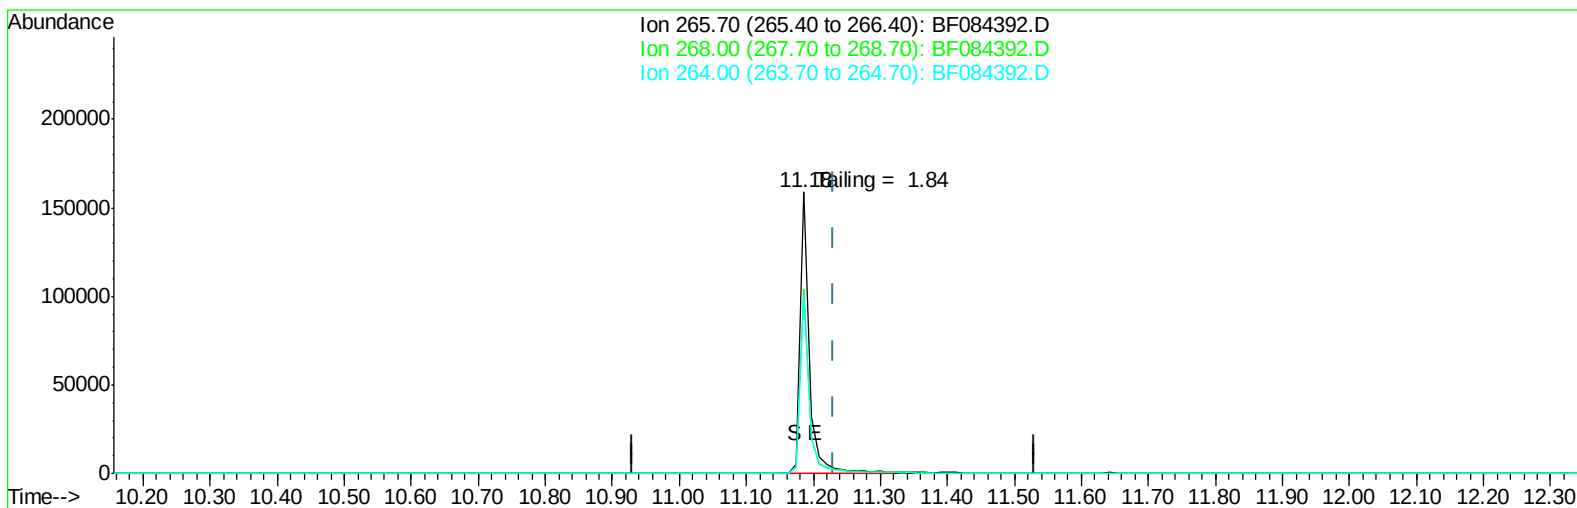

TIC: BF084392.D

(69) Pentachlorophenol (C)




11.185min (-0.045) 75551.37ng

response 154710

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	65.28
264.00	62.70	63.41
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
Data File : BF084392.D
Acq On : 11 Jan 2016 21:03
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 07:42:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

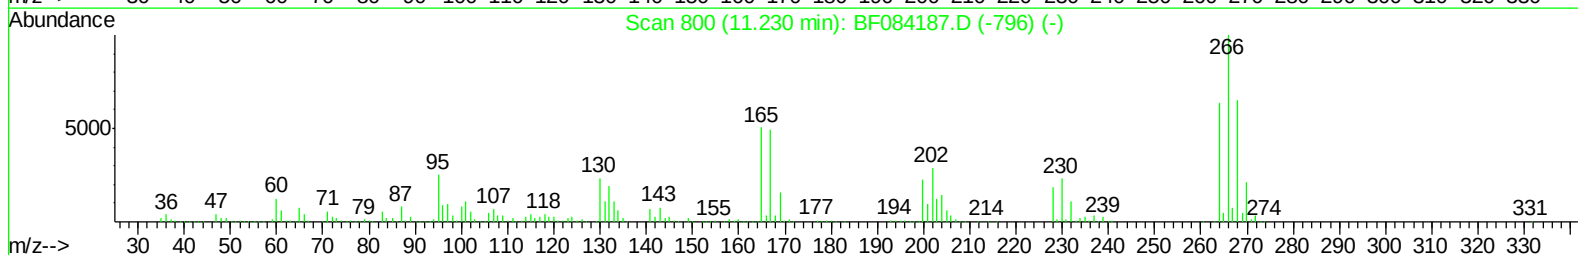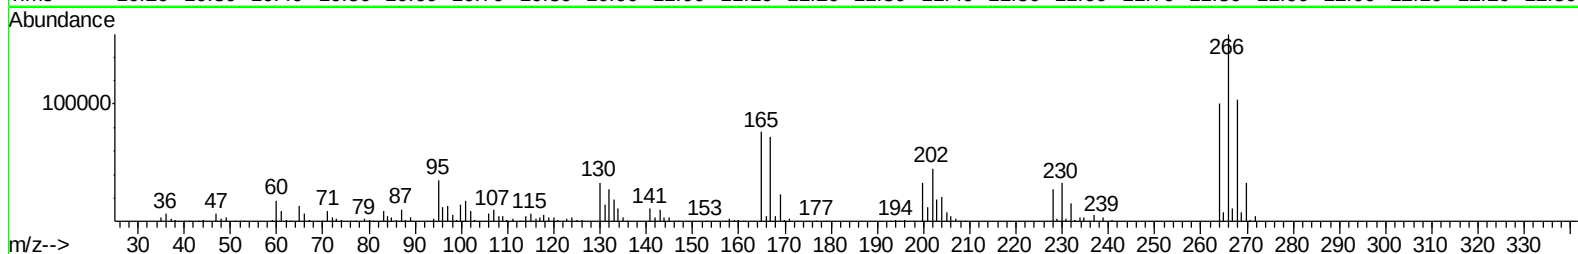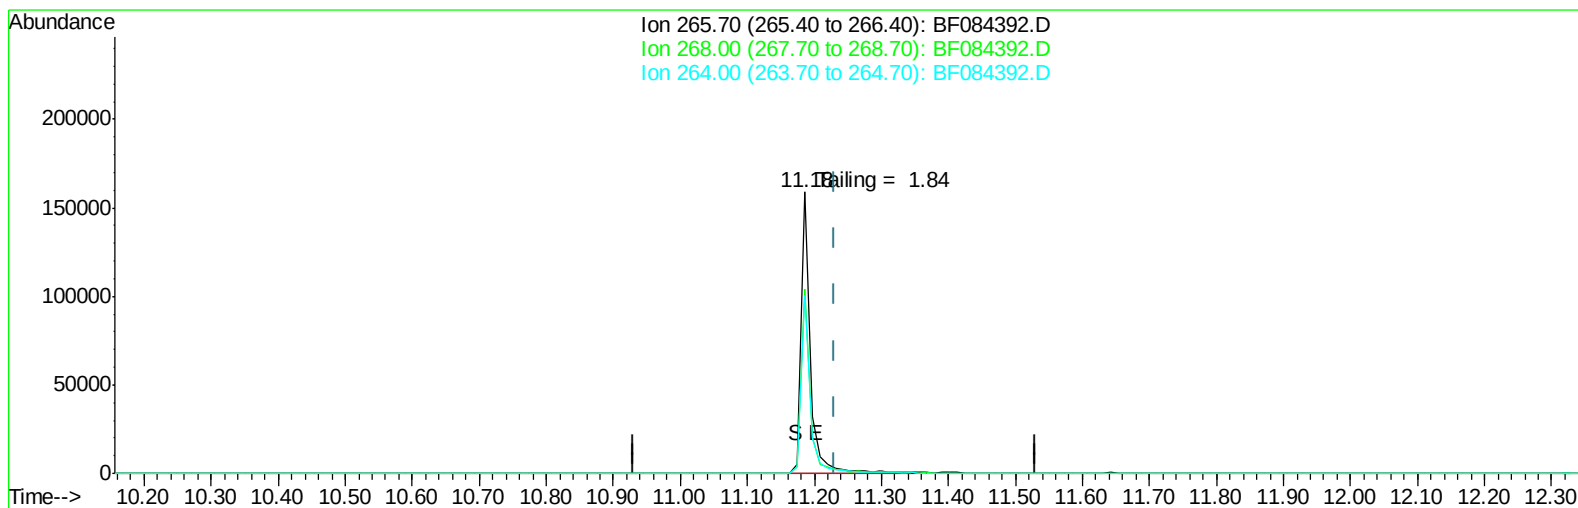

TIC: BF084392.D

(69) Pentachlorophenol (C)

11.185min (-0.045) 75551.37ng

response 154710

Ion	Exp%	Act%
265.70	100	100
268.00	65.50	65.28
264.00	62.70	63.41
0.00	0.00	0.00