

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
 Data File : BF084389.D
 Acq On : 11 Jan 2016 19:40
 Operator : SJ/UM
 Sample : H1065-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-12

Quant Time: Jan 12 11:17:05 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 04 12:22:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	399254	20.00	ng	-0.05
21) Naphthalene-d8	8.14	136	1555432	20.00	ng	-0.05
38) Acenaphthene-d10	9.89	164	699771	20.00	ng	-0.06
63) Phenanthrene-d10	11.38	188	1154520	20.00	ng	-0.05
75) Chrysene-d12	14.01	240	722022	20.00	ng	-0.06
86) Perylene-d12	15.44	264	634036	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	1577557	63.91	ng	-0.03
7) Phenol-d6	6.50	99	1495850	48.25	ng	-0.03
23) Nitrobenzene-d5	7.42	82	2514956	89.99	ng	-0.05
41) 2,4,6-Tribromophenol	10.68	330	812134	114.96	ng	-0.06
44) 2-Fluorobiphenyl	9.22	172	3169651	79.25	ng	-0.04
78) Terphenyl-d14	12.97	244	2586481	79.96	ng	-0.05


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
Data File : BF084389.D
Acq On : 11 Jan 2016 19:40
Operator : SJ/UM
Sample : H1065-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-12

Quant Time: Jan 12 11:17:05 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

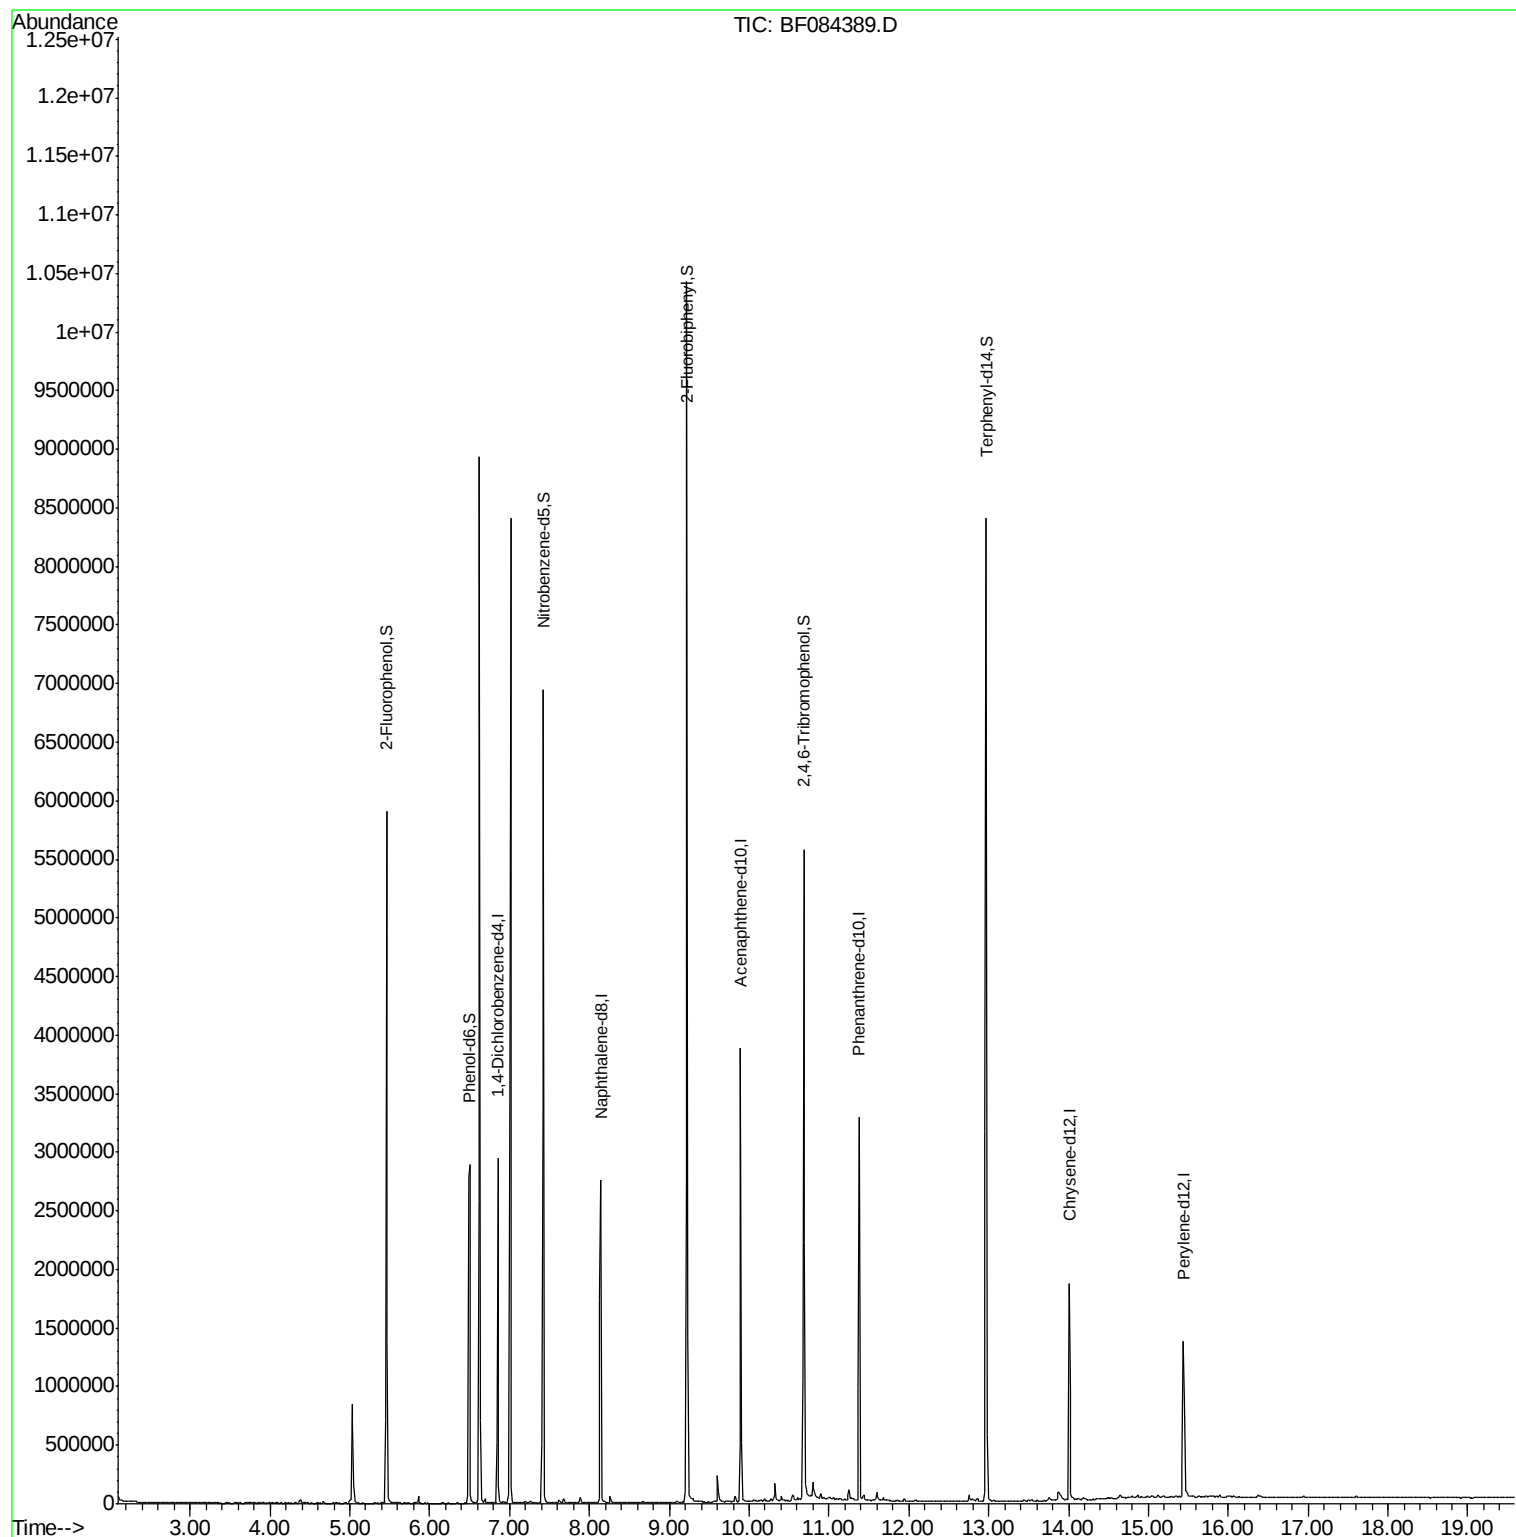



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 417

Delta R.T. -0.05 min

Lab File: BF084389.D

Acq: 11 Jan 2016 19:40

Instrument :

BNA_F

ClientSampled :

MW-12


Tgt Ion:152 Resp: 399254

Ion Ratio Lower Upper

152 100

150 156.8 123.0 184.4



115 63.6 51.4 77.2

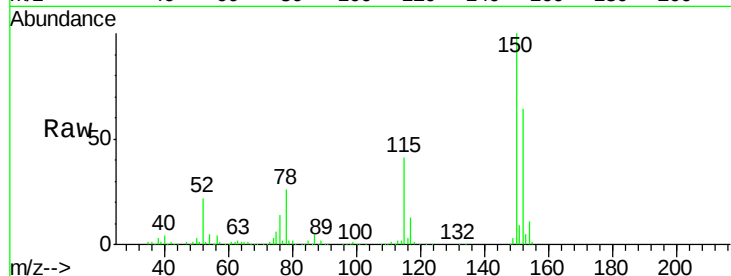

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

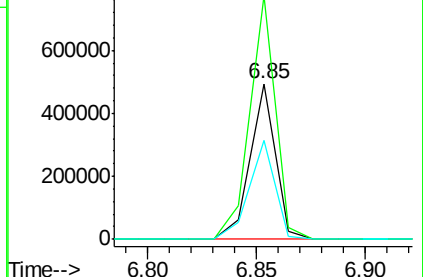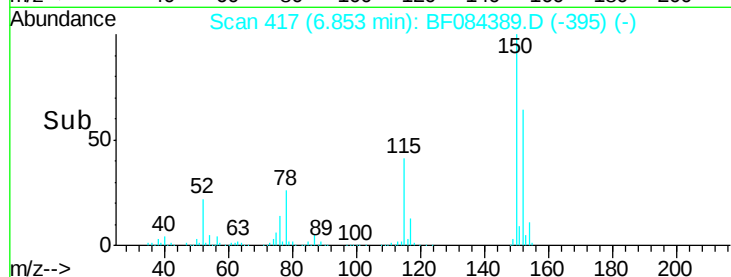

#5

2-Fluorophenol

Concen: 63.91 ng

RT: 5.46 min Scan# 295

Delta R.T. -0.03 min

Lab File: BF084389.D

Acq: 11 Jan 2016 19:40


Tgt Ion:112 Resp: 1577557

Ion Ratio Lower Upper

112 100

64 66.1 36.6 55.0#



63 33.6 19.4 29.0#

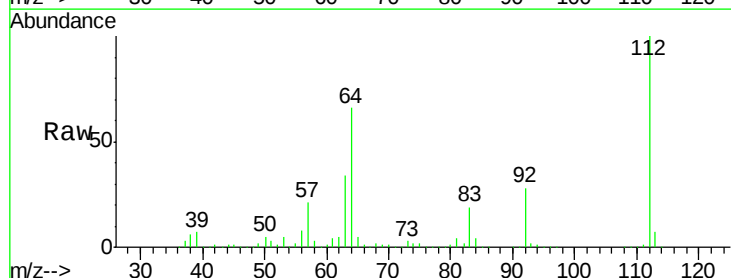

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

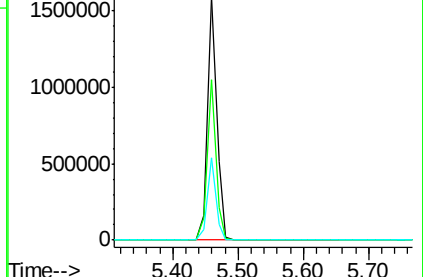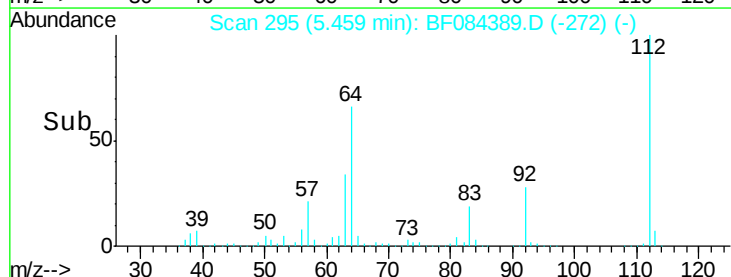



#7

Phenol-d6

Concen: 48.25 ng

RT: 6.50 min Scan# 386

Delta R.T. -0.03 min

Lab File: BF084389.D

Acq: 11 Jan 2016 19:40

Instrument :

BNA_F

ClientSampleId :

MW-12


Tgt Ion: 99 Resp: 1495850

Ion Ratio Lower Upper

99 100

42 12.9 12.8 19.2




71 27.2 30.9 46.3#

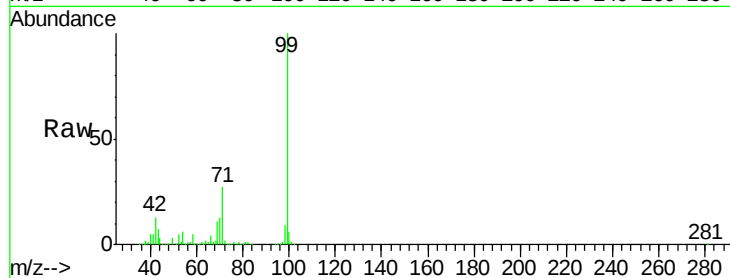

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

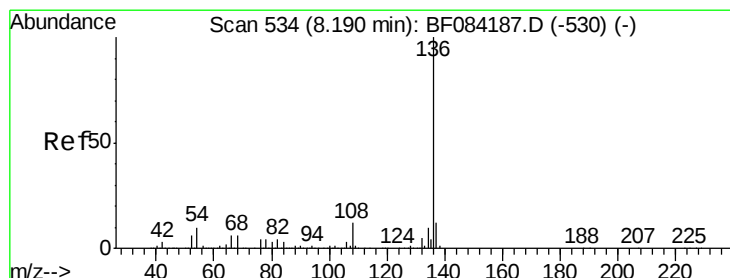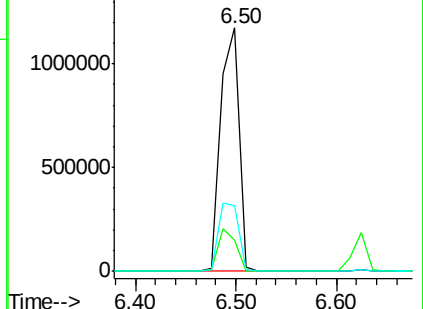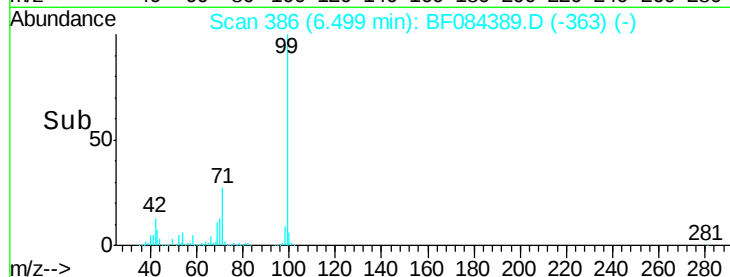

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 530

Delta R.T. -0.05 min

Lab File: BF084389.D

Acq: 11 Jan 2016 19:40

Tgt Ion: 136 Resp: 1555432


Ion Ratio Lower Upper

136 100

137 11.0 8.7 13.1

54 6.8 5.8 8.8

68 5.0 4.2 6.2


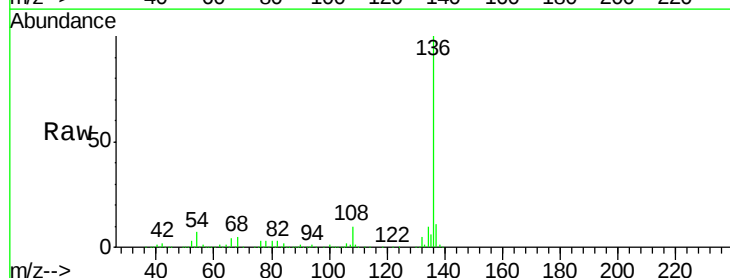


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

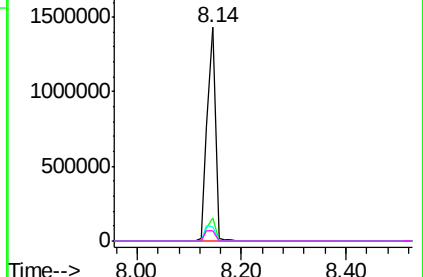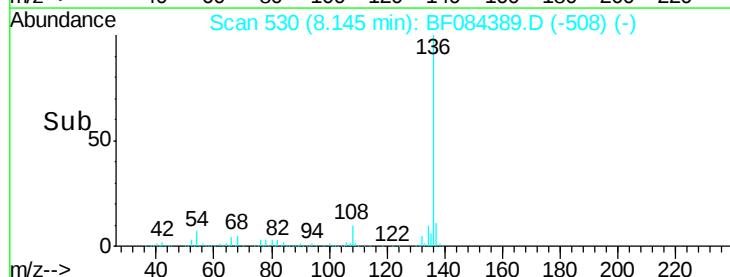







#23
Nitrobenzene-d5
Concen: 89.99 ng
RT: 7.42 min Scan# 467
Delta R.T. -0.05 min
Lab File: BF084389.D
Acq: 11 Jan 2016 19:40

Instrument :
BNA_F
ClientSampleId :
MW-12

Tgt Ion: 82 Resp: 2514956
Ion Ratio Lower Upper
82 100
128 47.4 34.6 51.8
54 55.9 38.4 57.6

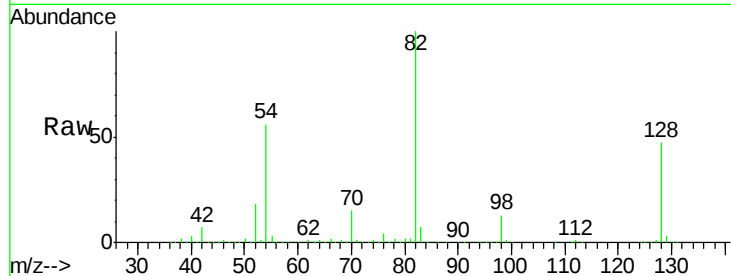


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

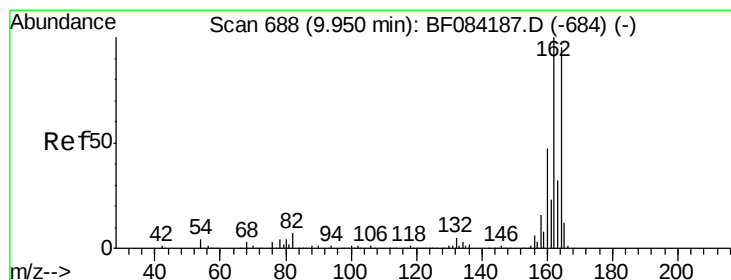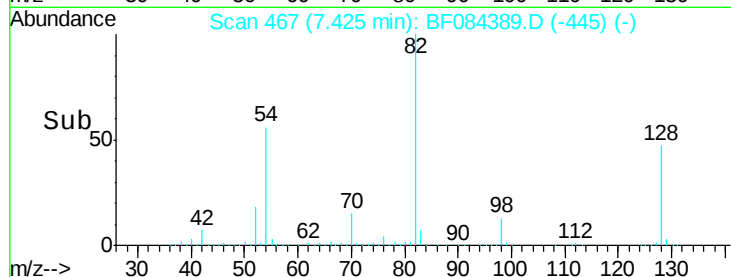
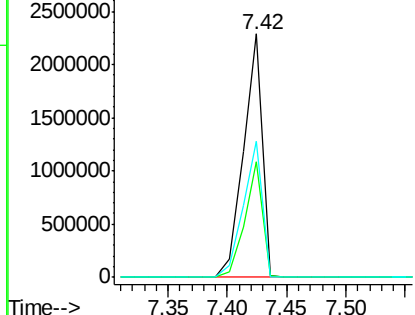


#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.89 min Scan# 683
Delta R.T. -0.06 min
Lab File: BF084389.D
Acq: 11 Jan 2016 19:40

Tgt Ion: 164 Resp: 699771
Ion Ratio Lower Upper
164 100
162 102.8 85.1 127.7
160 48.5 37.5 56.3

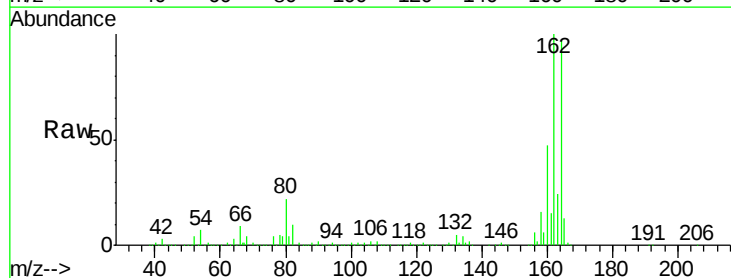

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

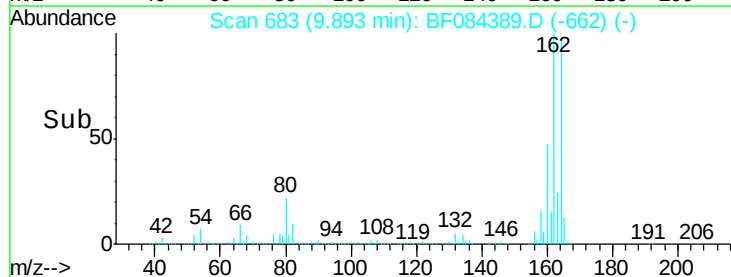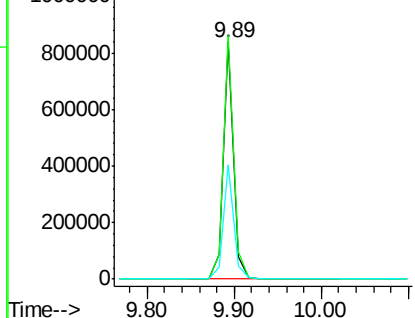







#41
 2,4,6-Tribromophenol
 Concen: 114.96 ng
 RT: 10.68 min Scan# 752
 Delta R.T. -0.06 min
 Lab File: BF084389.D
 Acq: 11 Jan 2016 19:40

Instrument :
 BNA_F
 ClientSampleId :
 MW-12

Tgt Ion:330 Resp: 812134
 Ion Ratio Lower Upper
 330 100
 332 96.4 76.6 114.8
 141 33.1 27.8 41.6

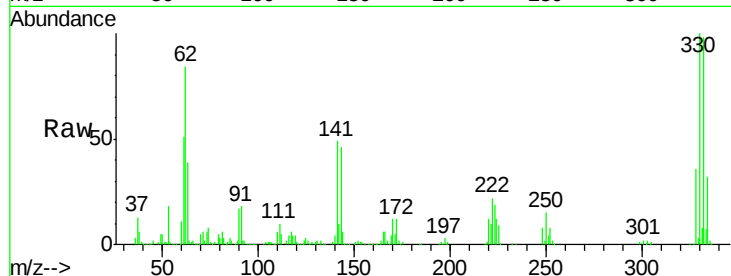


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

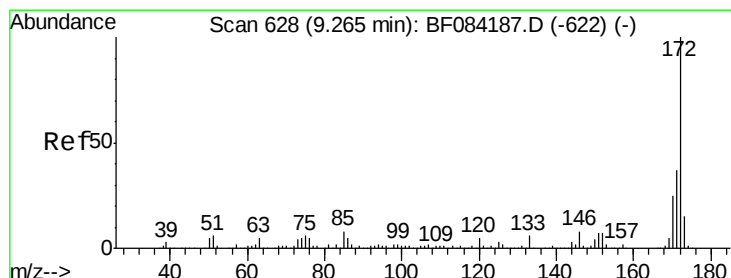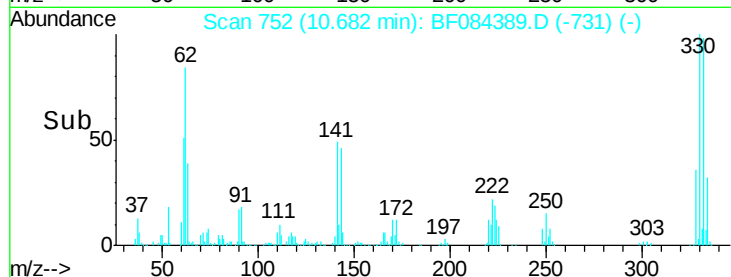
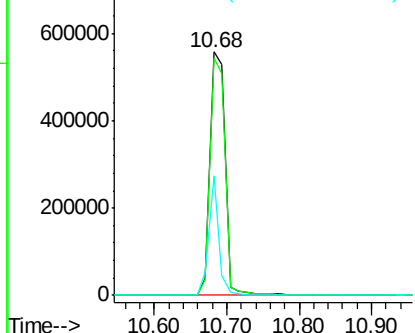



#44
 2-Fluorobiphenyl
 Concen: 79.25 ng
 RT: 9.22 min Scan# 624
 Delta R.T. -0.04 min
 Lab File: BF084389.D
 Acq: 11 Jan 2016 19:40

Tgt Ion:172 Resp: 3169651
 Ion Ratio Lower Upper
 172 100
 171 39.8 28.9 43.3
 170 27.6 18.6 27.8

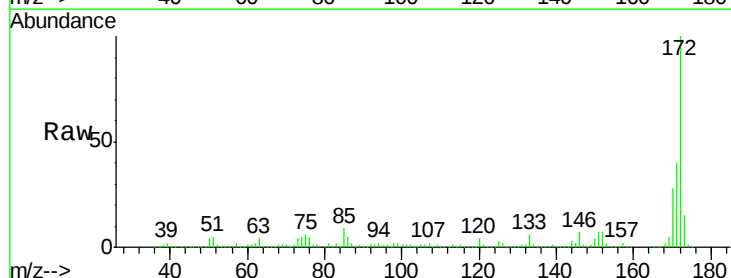

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

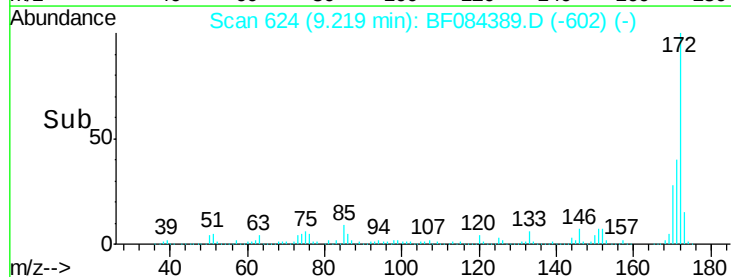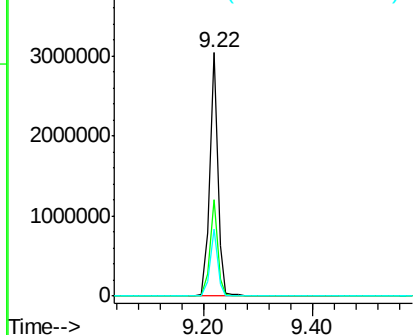

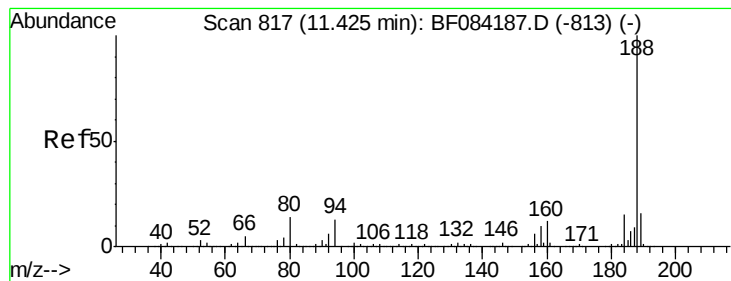

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.38 min Scan# 813

Delta R.T. -0.05 min

Lab File: BF084389.D

Acq: 11 Jan 2016 19:40

Instrument :

BNA_F

ClientSampleId :

MW-12


Tgt Ion:188 Resp: 1154520

Ion Ratio Lower Upper

188 100

94 10.0 9.0 13.4




80 10.1 9.6 14.4

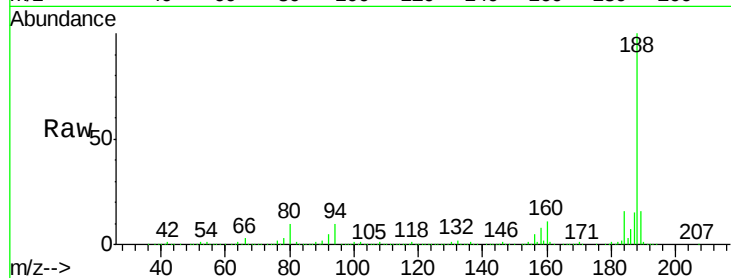

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

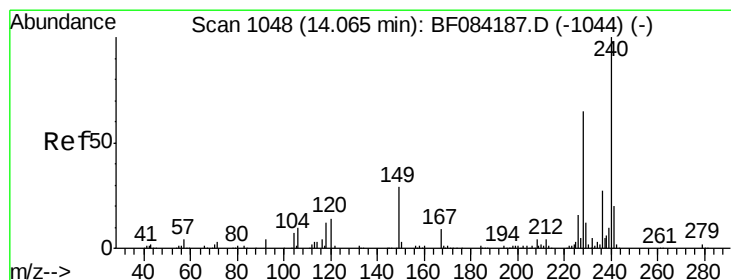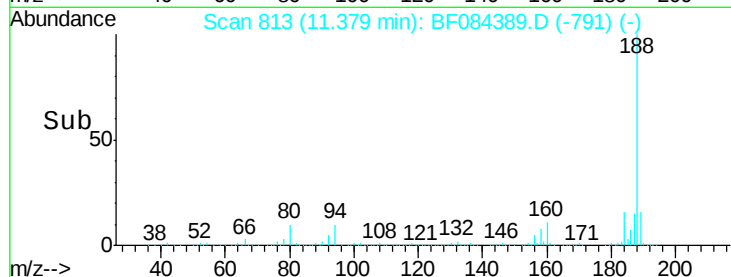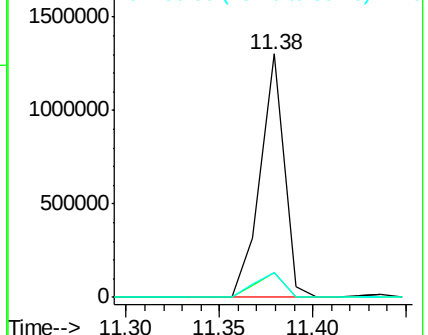

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.01 min Scan# 1043

Delta R.T. -0.06 min

Lab File: BF084389.D

Acq: 11 Jan 2016 19:40


Tgt Ion:240 Resp: 722022

Ion Ratio Lower Upper

240 100

120 18.4 9.5 14.3#



236 25.5 20.6 31.0

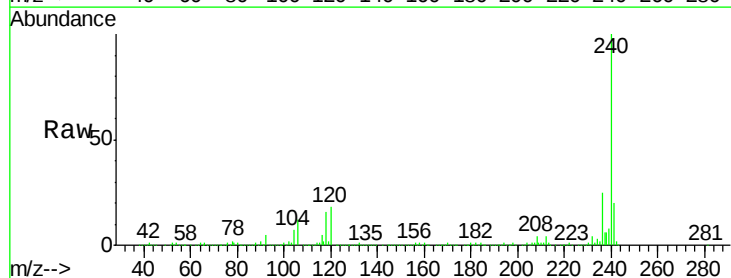


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

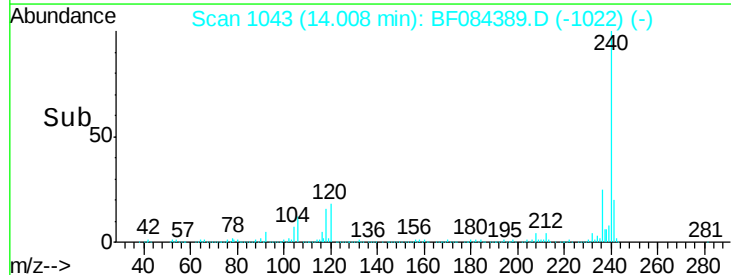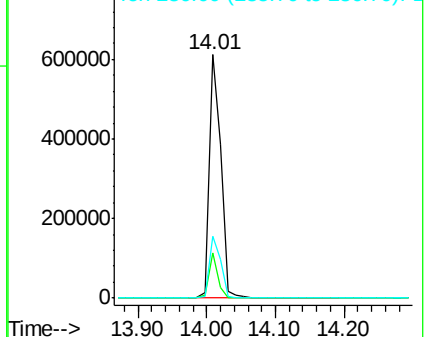

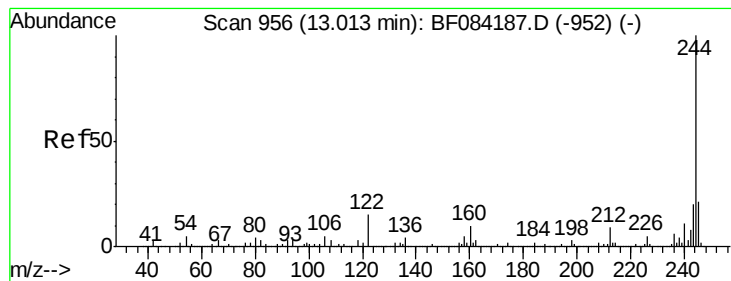

#78

Terphenyl-d14

Concen: 79.96 ng

RT: 12.97 min Scan# 952

Delta R.T. -0.05 min

Lab File: BF084389.D

Acq: 11 Jan 2016 19:40

Instrument :

BNA_F

ClientSampleId :

MW-12


Tgt Ion:244 Resp: 2586481

Ion Ratio Lower Upper

244 100

212 8.0 5.7 8.5




122 14.3 7.4 11.0#

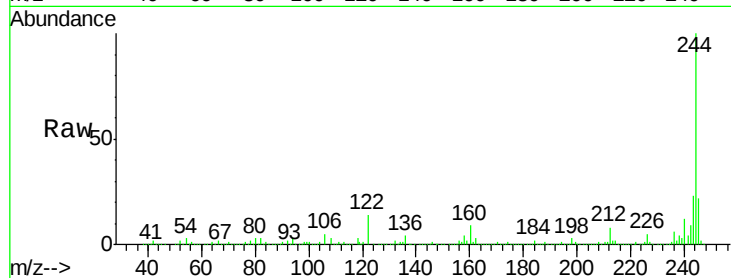

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

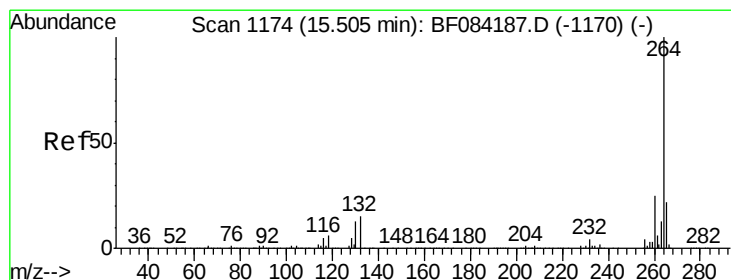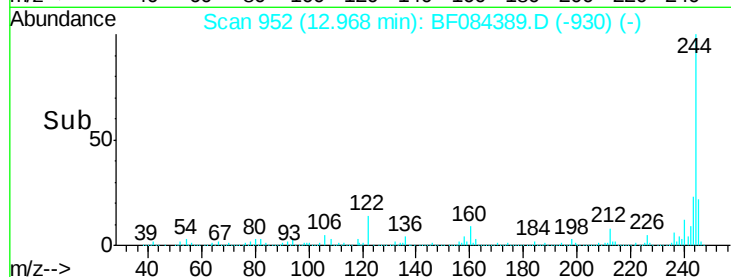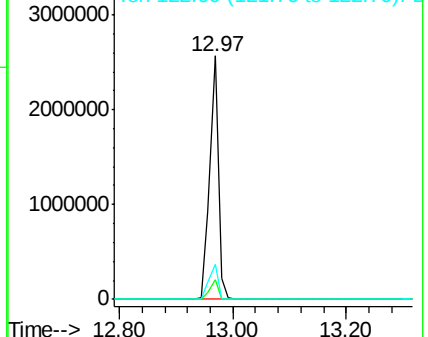

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.44 min Scan# 1168

Delta R.T. -0.07 min

Lab File: BF084389.D

Acq: 11 Jan 2016 19:40


Tgt Ion:264 Resp: 634036

Ion Ratio Lower Upper

264 100

260 23.5 19.4 29.2

265 21.5 17.8 26.6

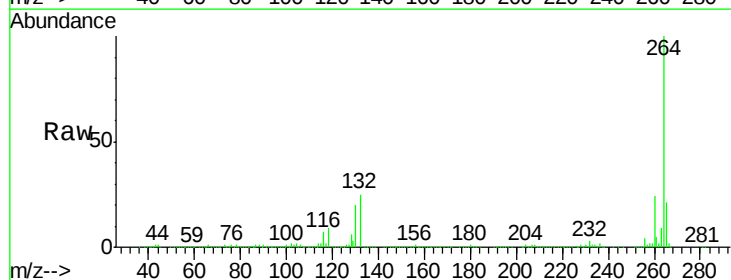

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

