

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
 Data File : BF084408.D
 Acq On : 12 Jan 2016 5:04
 Operator : SJ/UM
 Sample : H1067-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-03

Quant Time: Jan 12 06:48:42 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 04 12:22:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	364565	20.00	ng	-0.05
21) Naphthalene-d8	8.14	136	1395290	20.00	ng	-0.05
38) Acenaphthene-d10	9.89	164	625358	20.00	ng	-0.06
63) Phenanthrene-d10	11.38	188	972077	20.00	ng	-0.05
75) Chrysene-d12	14.02	240	682553	20.00	ng	-0.05
86) Perylene-d12	15.44	264	584730	20.00	ng	-0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	1363005	60.47	ng	-0.03
7) Phenol-d6	6.50	99	1178443	41.63	ng	-0.03
23) Nitrobenzene-d5	7.42	82	2335888	93.17	ng	-0.05
41) 2,4,6-Tribromophenol	10.69	330	817614	129.50	ng	-0.05
44) 2-Fluorobiphenyl	9.22	172	3017946	84.89	ng	-0.05
78) Terphenyl-d14	12.97	244	1976166	64.63	ng	-0.05


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
Data File : BF084408.D
Acq On : 12 Jan 2016 5:04
Operator : SJ/UM
Sample : H1067-05
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-03

Quant Time: Jan 12 06:48:42 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 04 12:22:40 2016
Response via : Initial Calibration

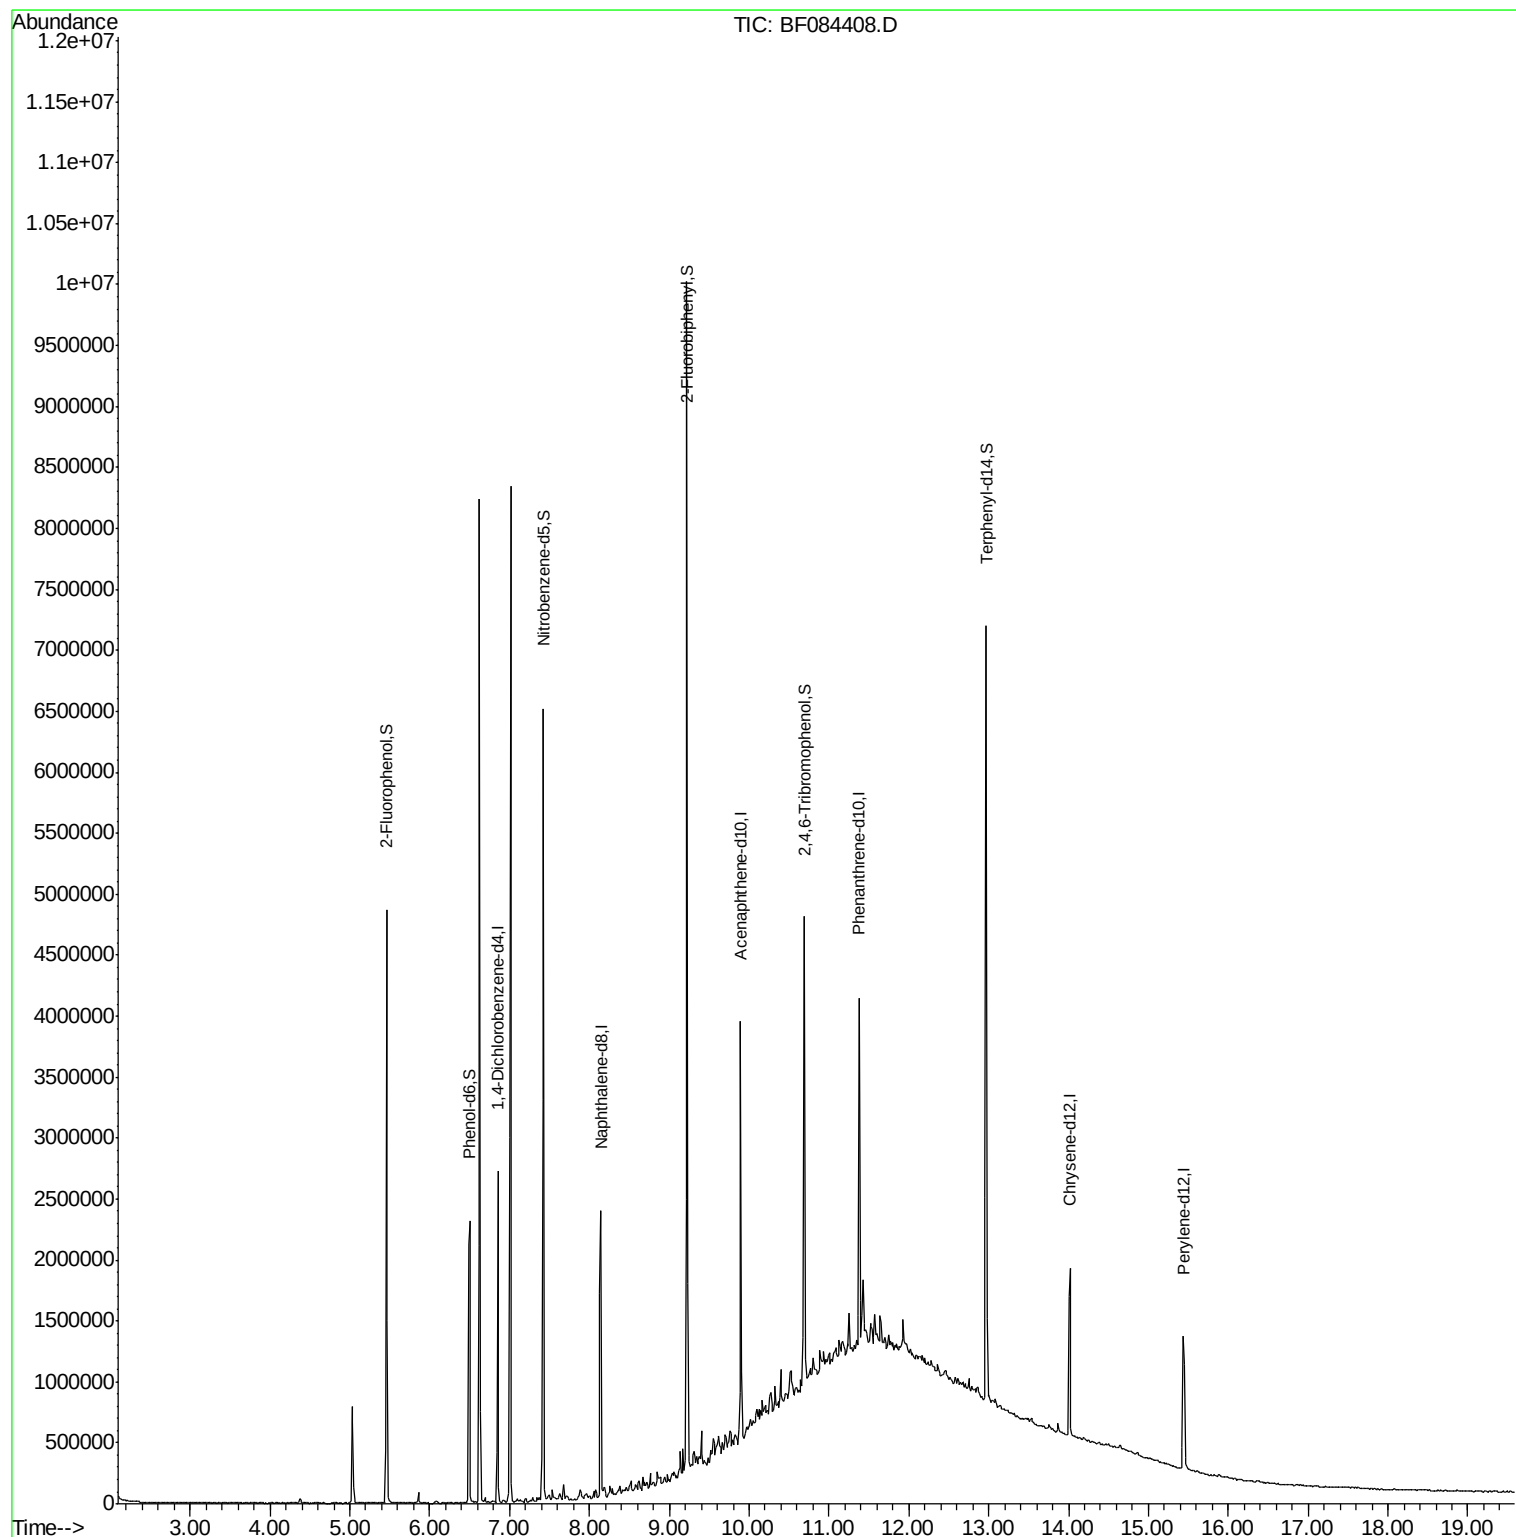

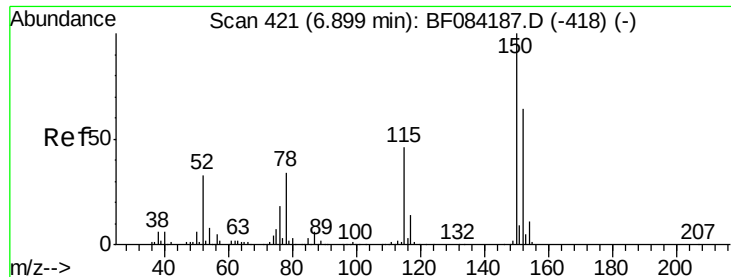

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.85 min Scan# 417

Delta R.T. -0.05 min

Lab File: BF084408.D

Acq: 12 Jan 2016 5:04

Instrument :

BNA_F

ClientSampleId :

MW-03


Tgt Ion:152 Resp: 364565

Ion Ratio Lower Upper

152 100

150 155.1 123.0 184.4




115 62.4 51.4 77.2

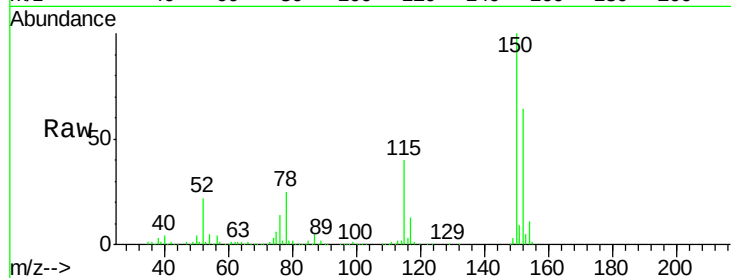

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

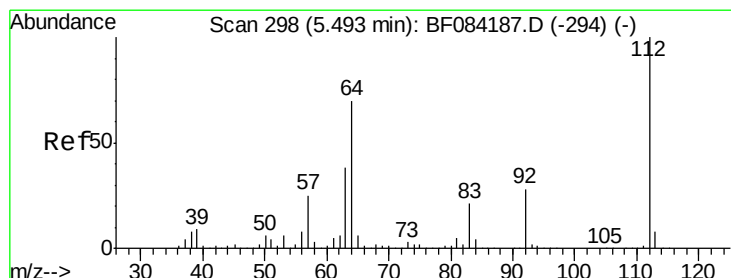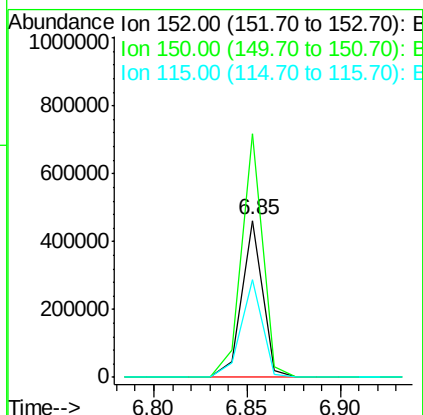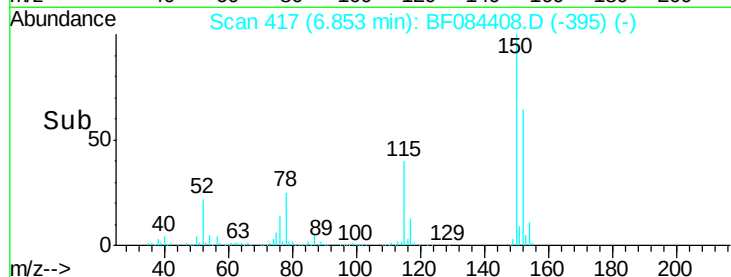

#5

2-Fluorophenol

Concen: 60.47 ng

RT: 5.46 min Scan# 295

Delta R.T. -0.03 min

Lab File: BF084408.D

Acq: 12 Jan 2016 5:04


Tgt Ion:112 Resp: 1363005

Ion Ratio Lower Upper

112 100

64 66.6 36.6 55.0#



63 33.8 19.4 29.0#

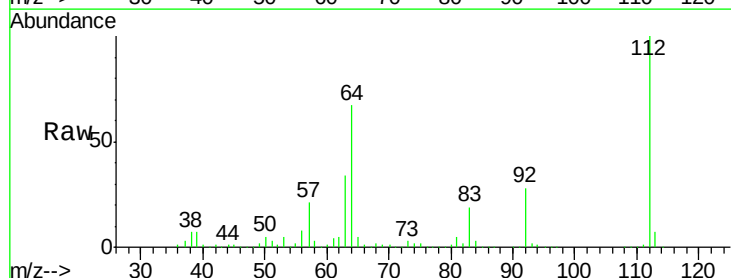


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

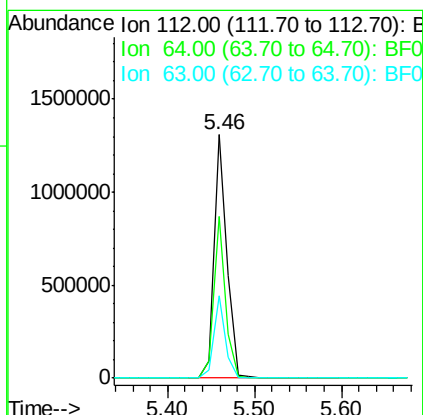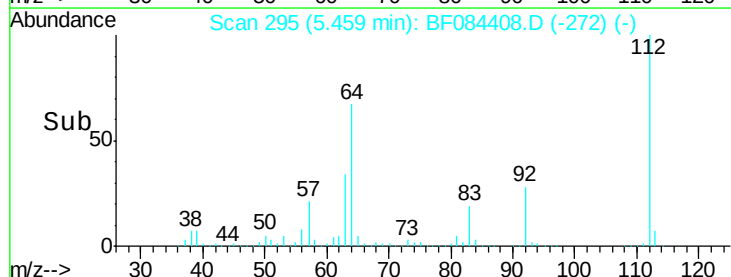

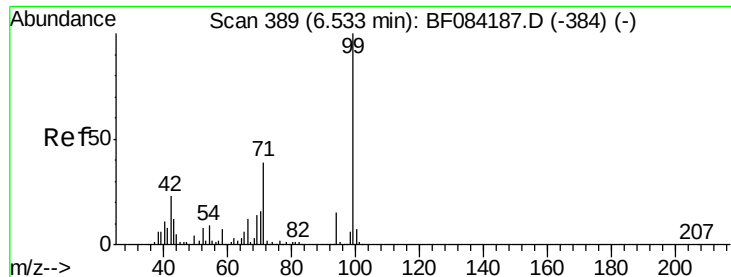

#7

Phenol-d6

Concen: 41.63 ng

RT: 6.50 min Scan# 386

Delta R.T. -0.03 min

Lab File: BF084408.D

Acq: 12 Jan 2016 5:04

Instrument :

BNA_F

ClientSampleId :

MW-03


Tgt Ion: 99 Resp: 1178443

Ion Ratio Lower Upper




99 100

42 12.9 12.8 19.2

71 26.9 30.9 46.3#

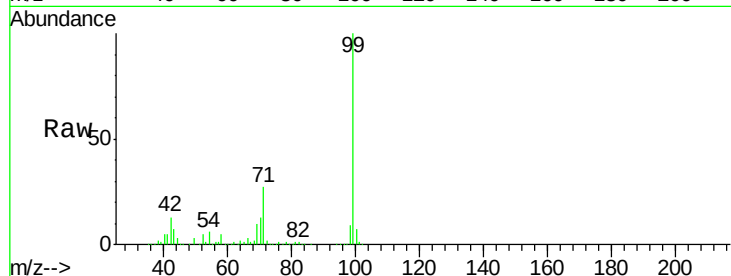

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

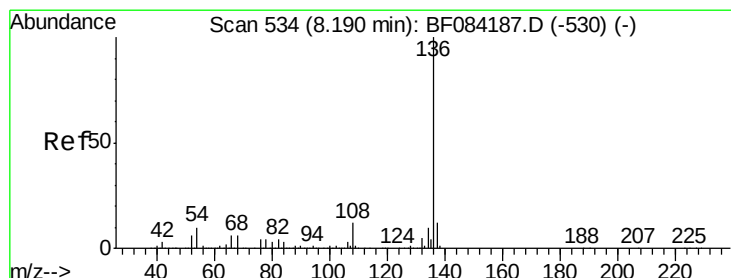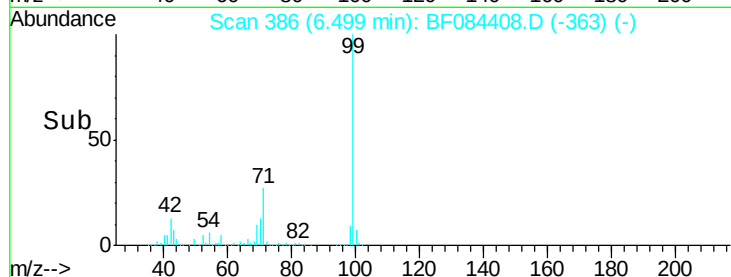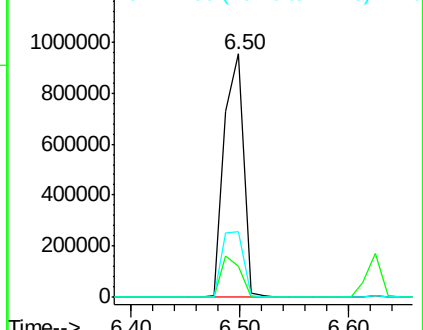

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.14 min Scan# 530

Delta R.T. -0.05 min

Lab File: BF084408.D

Acq: 12 Jan 2016 5:04

Tgt Ion: 136 Resp: 1395290


Ion Ratio Lower Upper

136 100



137 11.1 8.7 13.1


54 6.5 5.8 8.8

68 4.8 4.2 6.2

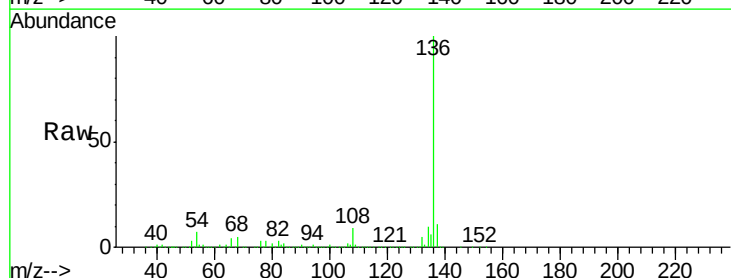

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

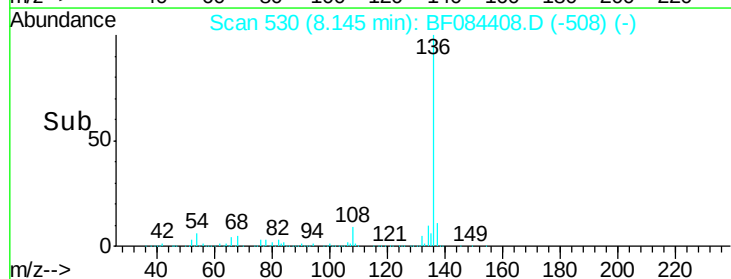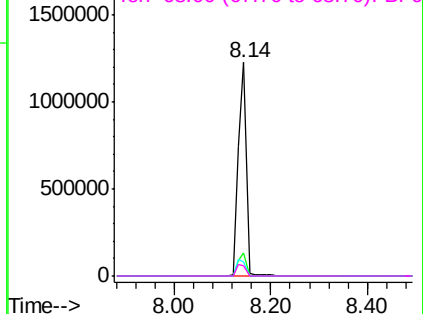


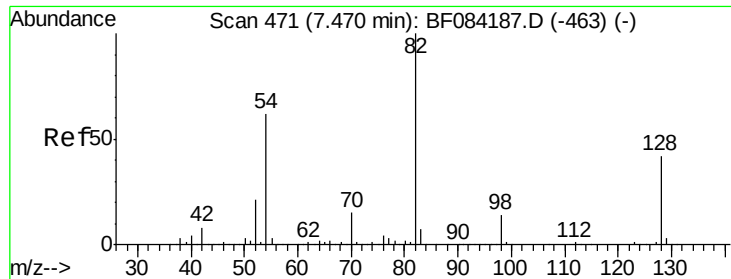




#23
 Nitrobenzene-d5
 Concen: 93.17 ng
 RT: 7.42 min Scan# 467
 Delta R.T. -0.05 min
 Lab File: BF084408.D
 Acq: 12 Jan 2016 5:04

Instrument :
 BNA_F
 ClientSampleId :
 MW-03

Tgt Ion: 82 Resp: 2335888
 Ion Ratio Lower Upper
 82 100
 128 46.5 34.6 51.8
 54 56.2 38.4 57.6

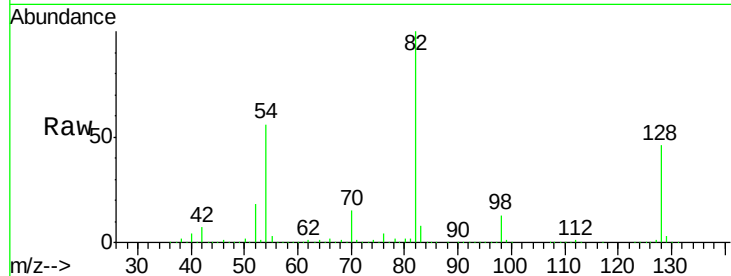


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

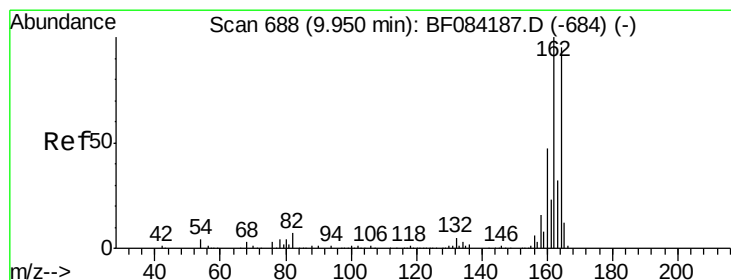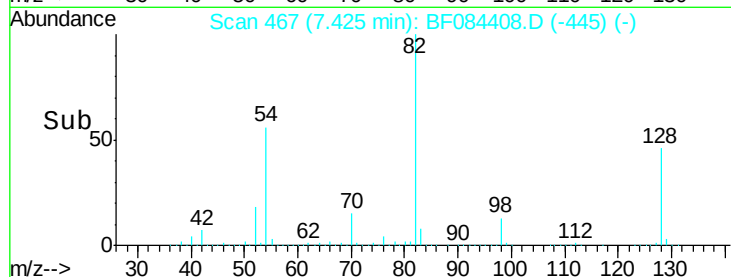
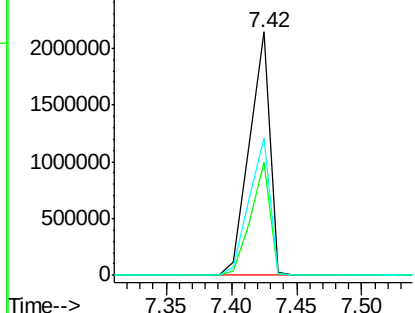



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.89 min Scan# 683
 Delta R.T. -0.06 min
 Lab File: BF084408.D
 Acq: 12 Jan 2016 5:04

Tgt Ion: 164 Resp: 625358
 Ion Ratio Lower Upper
 164 100
 162 102.4 85.1 127.7
 160 46.1 37.5 56.3

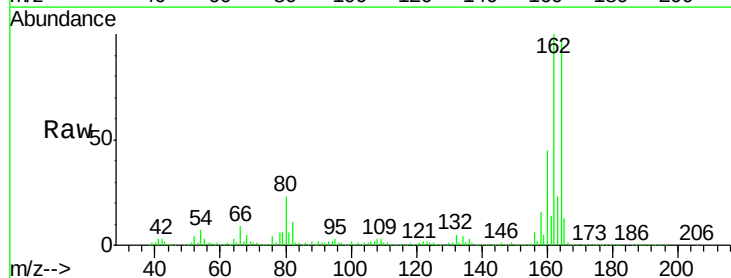

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

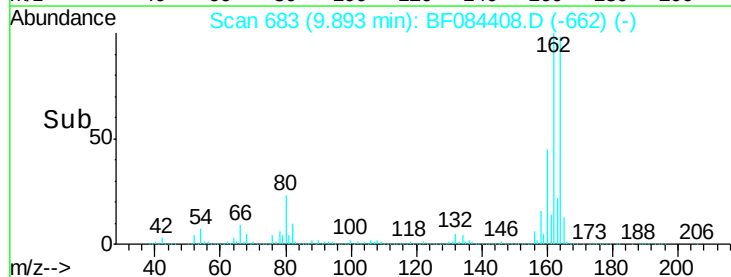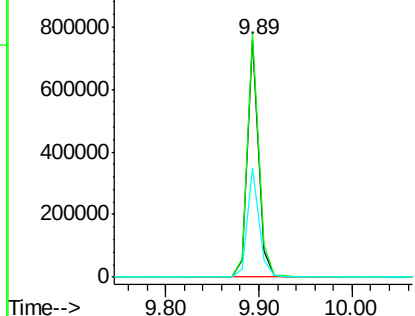


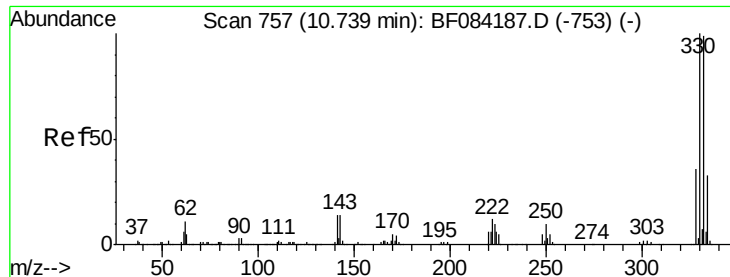




#41
 2,4,6-Tribromophenol
 Concen: 129.50 ng
 RT: 10.69 min Scan# 753
 Delta R.T. -0.05 min
 Lab File: BF084408.D
 Acq: 12 Jan 2016 5:04

Instrument :
 BNA_F
 ClientSampleId :
 MW-03

Tgt Ion:330 Resp: 817614
 Ion Ratio Lower Upper
 330 100
 332 96.7 76.6 114.8
 141 31.7 27.8 41.6

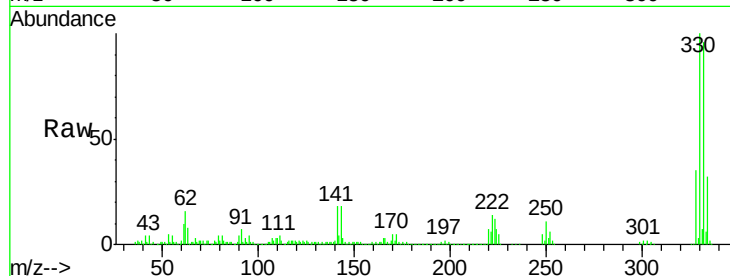


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

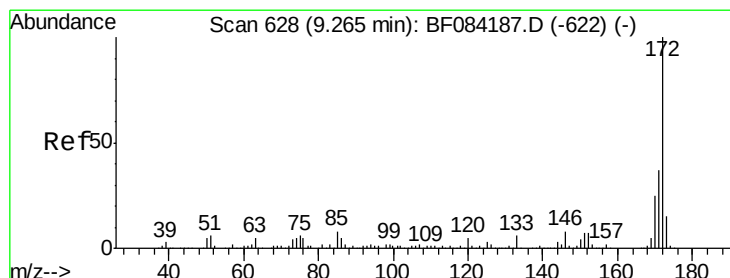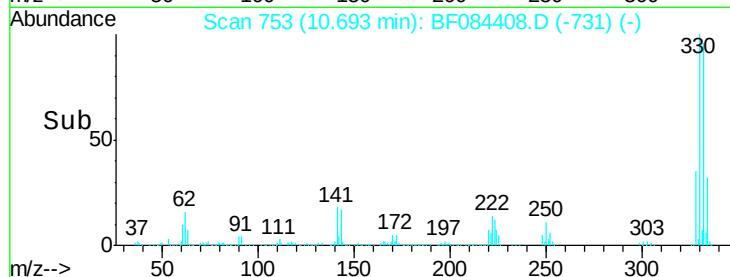
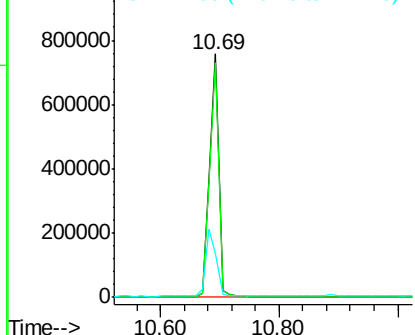



#44
 2-Fluorobiphenyl
 Concen: 84.89 ng
 RT: 9.22 min Scan# 624
 Delta R.T. -0.05 min
 Lab File: BF084408.D
 Acq: 12 Jan 2016 5:04

Tgt Ion:172 Resp: 3017946
 Ion Ratio Lower Upper
 172 100
 171 39.9 28.9 43.3
 170 27.2 18.6 27.8

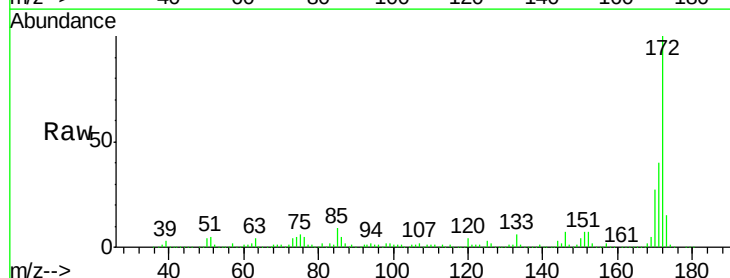

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

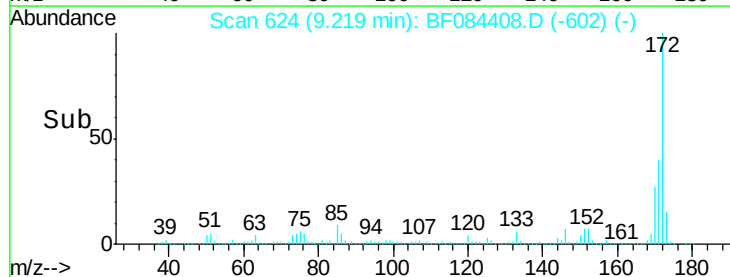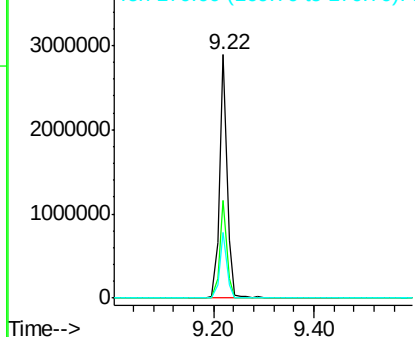

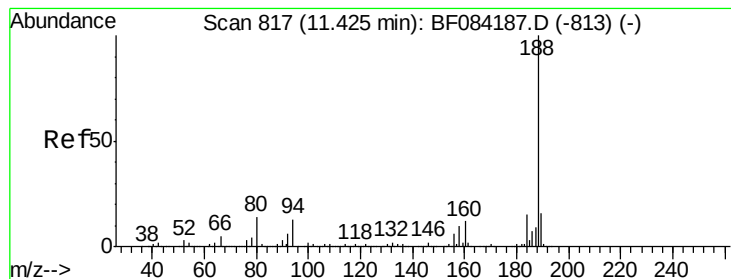

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.38 min Scan# 813

Delta R.T. -0.05 min

Lab File: BF084408.D

Acq: 12 Jan 2016 5:04

Instrument :

BNA_F

ClientSampleId :

MW-03


Tgt Ion:188 Resp: 972077

Ion Ratio Lower Upper

188 100

94 12.7 9.0 13.4




80 12.9 9.6 14.4

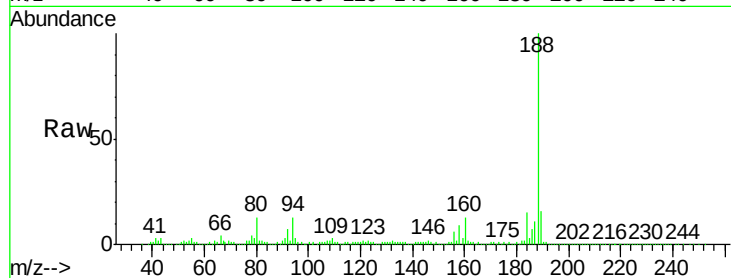

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

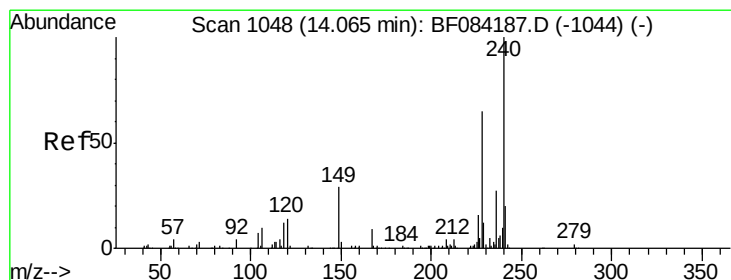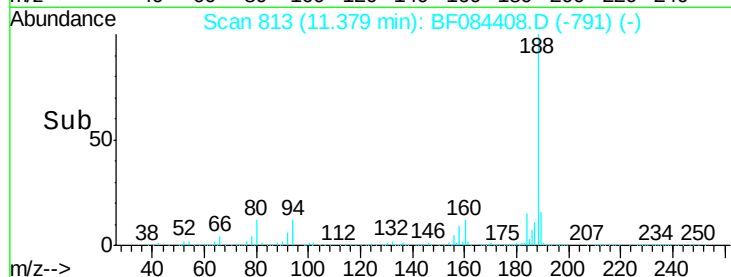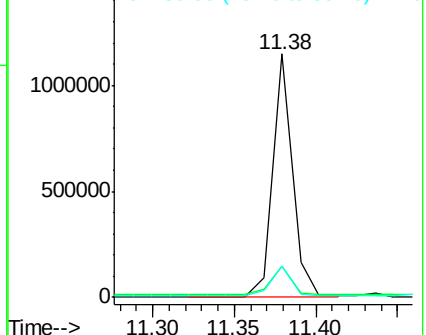

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.02 min Scan# 1044

Delta R.T. -0.05 min

Lab File: BF084408.D

Acq: 12 Jan 2016 5:04


Tgt Ion:240 Resp: 682553

Ion Ratio Lower Upper

240 100

120 8.6 9.5 14.3#



236 25.8 20.6 31.0

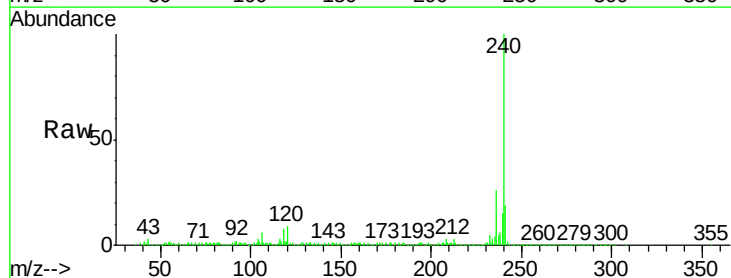


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

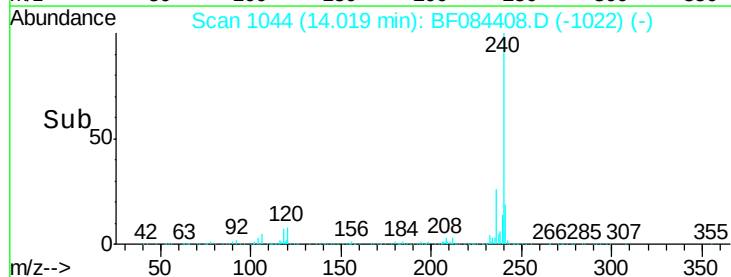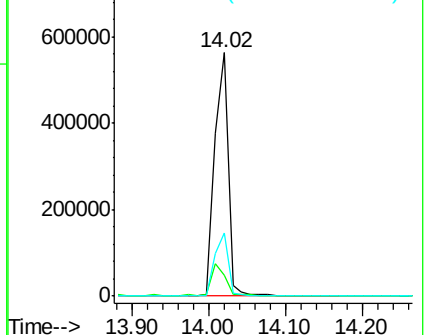

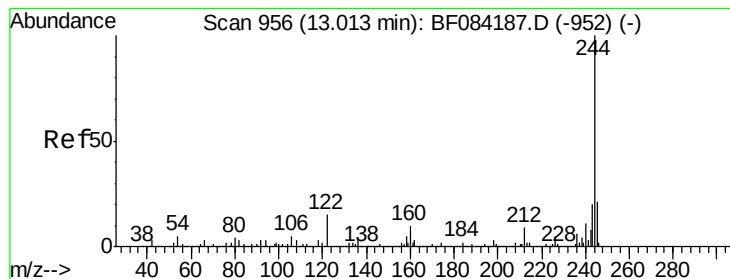

#78

Terphenyl-d14

Concen: 64.63 ng

RT: 12.97 min Scan# 952

Delta R.T. -0.05 min

Lab File: BF084408.D

Acq: 12 Jan 2016 5:04

Instrument :

BNA_F

ClientSampleId :

MW-03


Tgt Ion:244 Resp: 1976166

Ion Ratio Lower Upper

244 100

212 7.8 5.7 8.5




122 14.1 7.4 11.0#

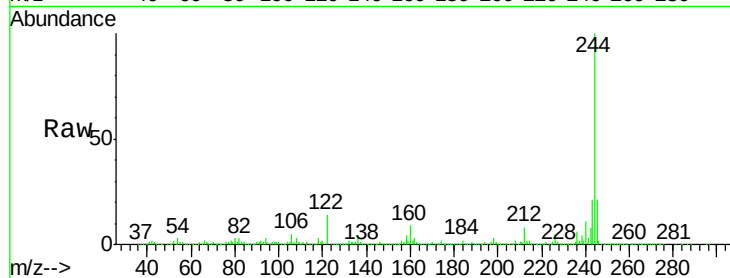

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

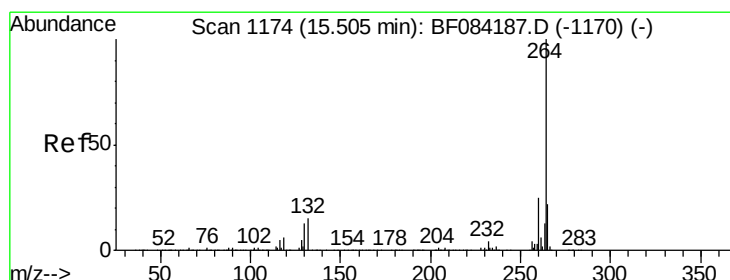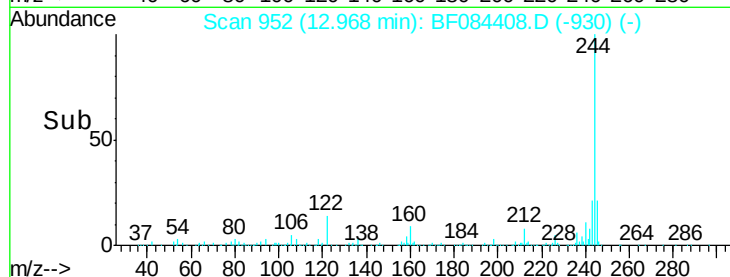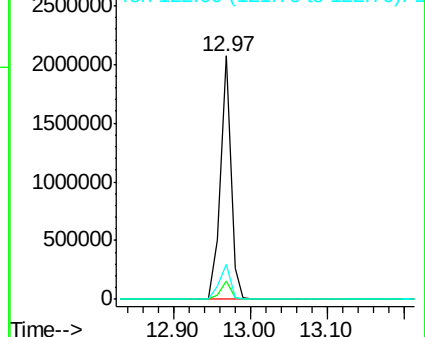

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.44 min Scan# 1168

Delta R.T. -0.07 min

Lab File: BF084408.D

Acq: 12 Jan 2016 5:04


Tgt Ion:264 Resp: 584730

Ion Ratio Lower Upper

264 100

260 23.6 19.4 29.2

265 22.1 17.8 26.6

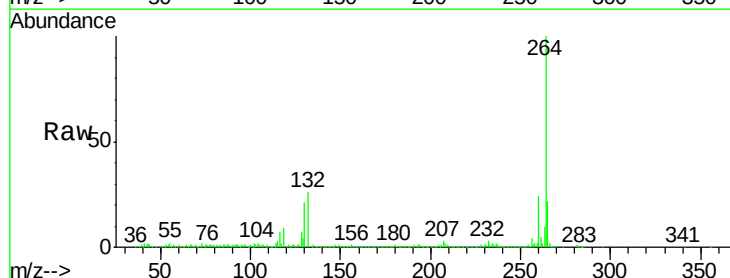

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

