


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
Data File : BF084371.D
Acq On : 11 Jan 2016 8:55
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jan 04 12:22:40 2016

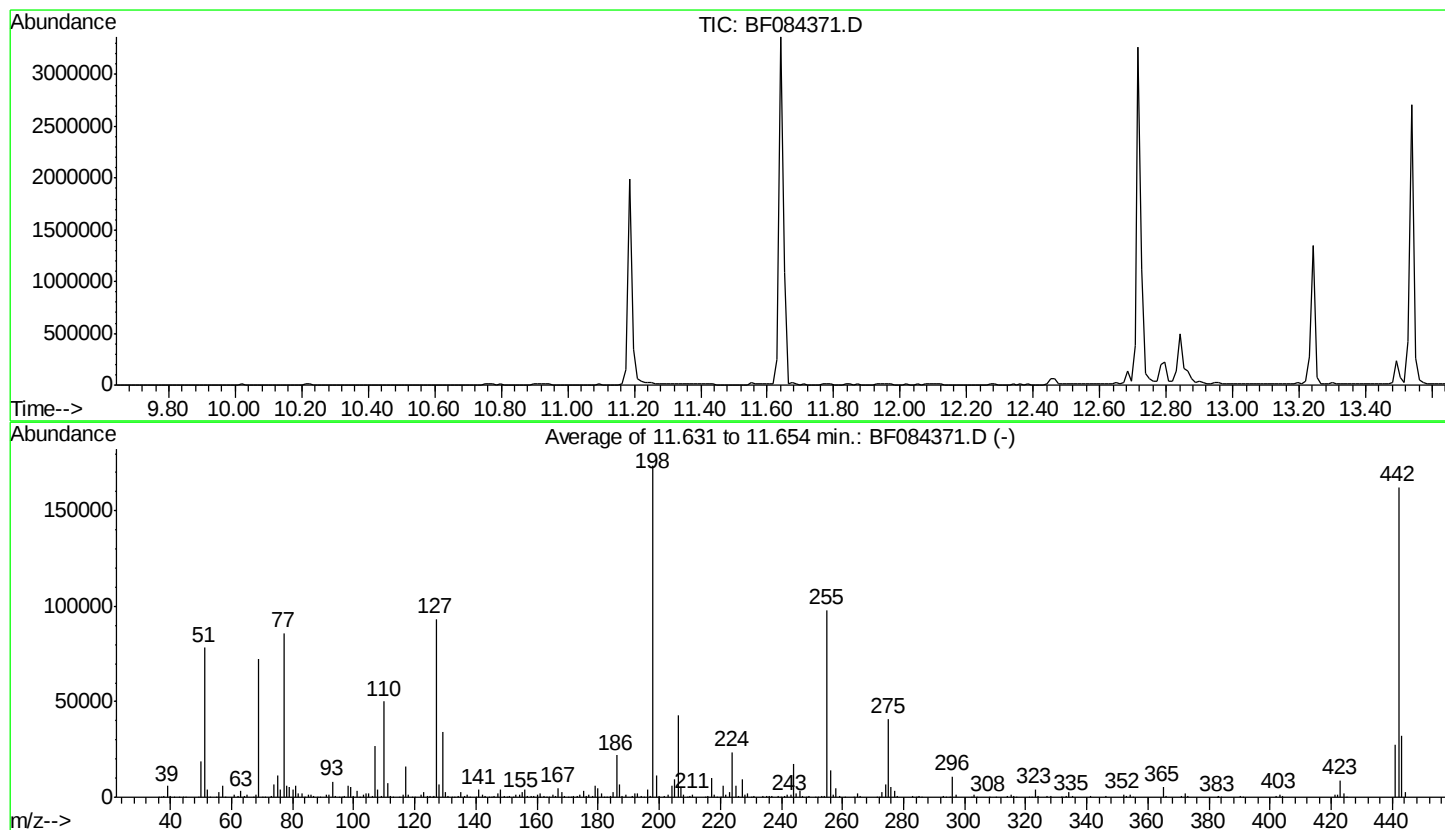

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	78379	PASS
68	69	0.00	2	1.5	1067	PASS
69	198	0.00	100	41.5	72121	PASS
70	69	0.00	2	0.5	327	PASS
127	198	10	80	53.7	93184	PASS
197	198	0.00	2	0.3	508	PASS
198	198	100	100	100.0	173648	PASS
199	198	5	9	6.5	11240	PASS
275	198	10	60	23.7	41224	PASS
365	198	1	100	3.2	5487	PASS
441	442	0.01	24	16.9	27482	PASS
442	198	50	100	93.6	162570	PASS
443	442	15	24	19.7	32000	PASS