


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF011116\
 Data File : BF084392.D
 Acq On : 11 Jan 2016 21:03
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF123115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 04 12:22:40 2016

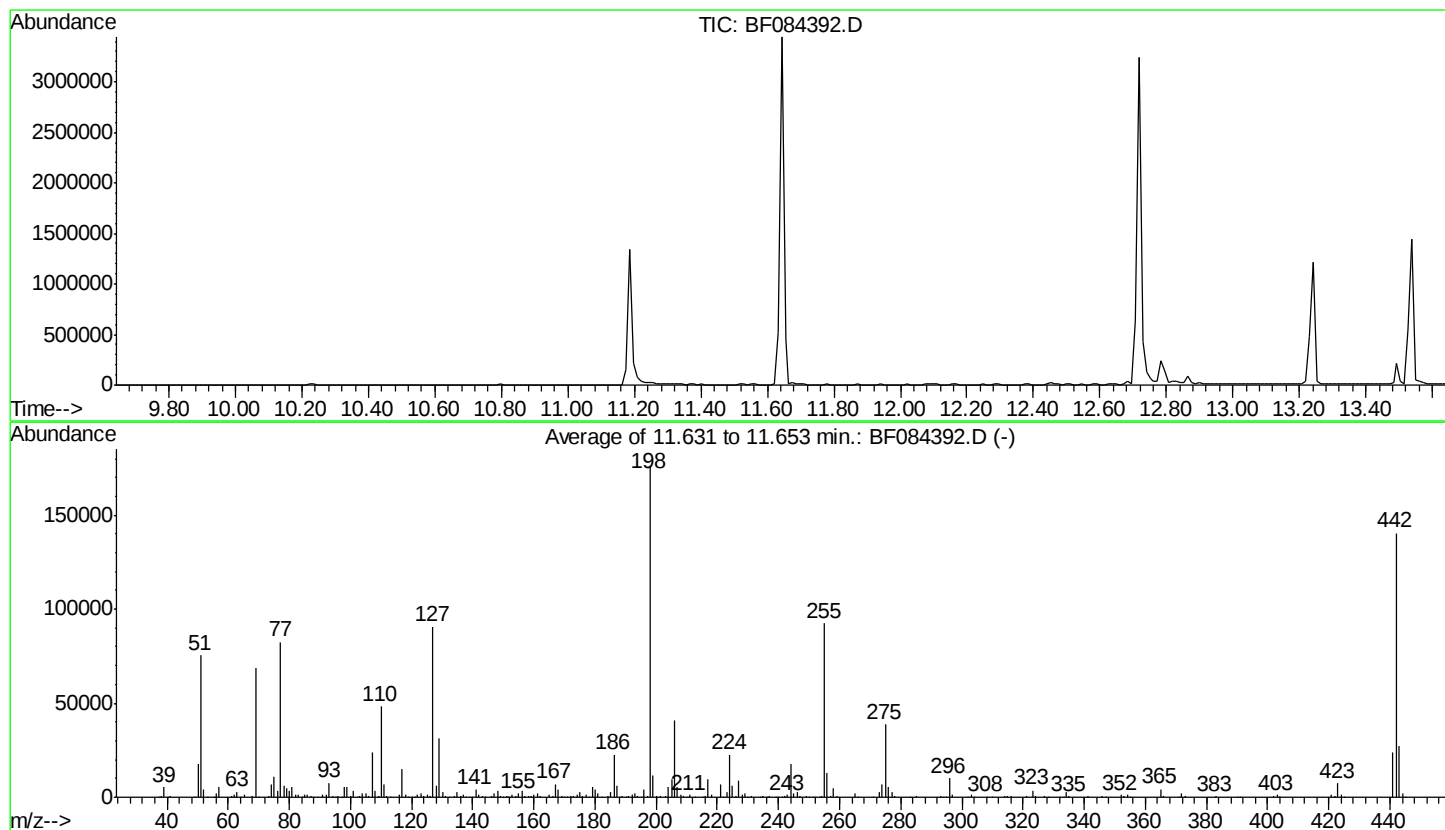

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	75281	PASS
68	69	0.00	2	1.5	1032	PASS
69	198	0.00	100	38.9	68543	PASS
70	69	0.00	2	0.4	250	PASS
127	198	10	80	51.5	90858	PASS
197	198	0.00	2	0.5	891	PASS
198	198	100	100	100.0	176322	PASS
199	198	5	9	6.6	11634	PASS
275	198	10	60	22.0	38754	PASS
365	198	1	100	2.5	4441	PASS
441	442	0.01	24	17.0	23877	PASS
442	198	50	100	79.7	140561	PASS
443	442	15	24	19.2	26965	PASS