
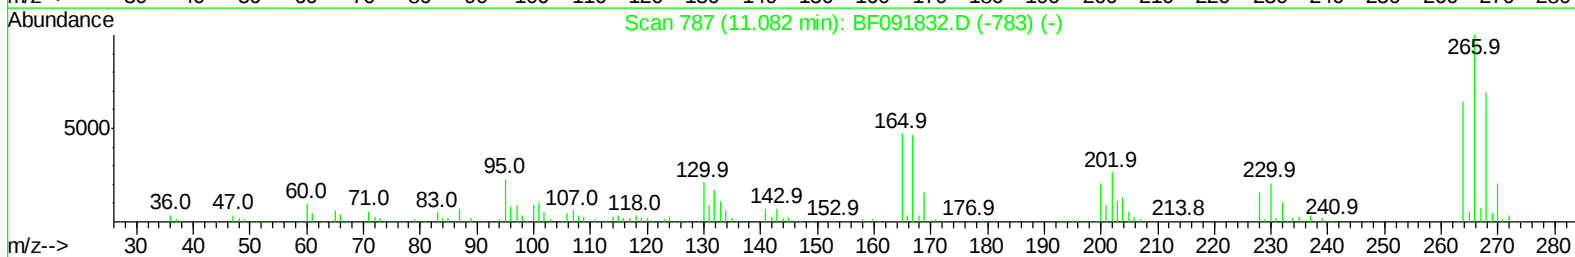
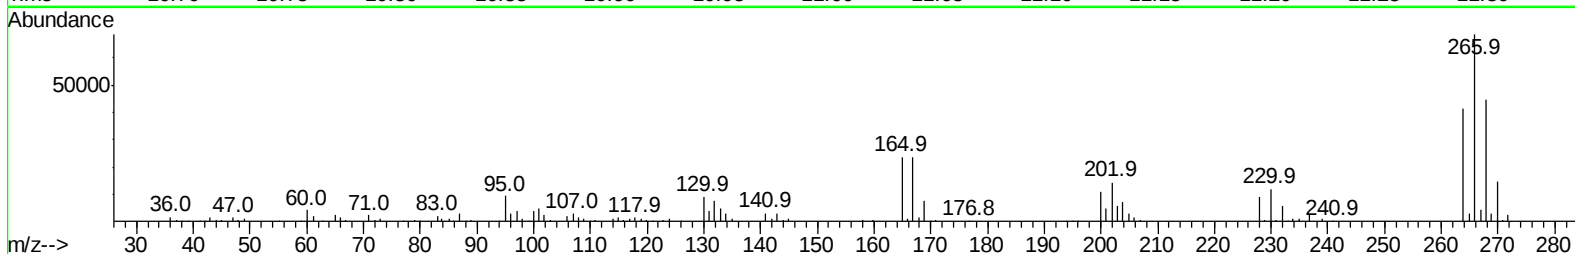


Data Path : Z:\HPCHEM1\BNA F\Data\BF011117\
 Data File : BF092199.D
 Acq On : 11 Jan 2017 15:07
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 14:27:49 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 06 15:43:51 2017
 Response via : Initial Calibration

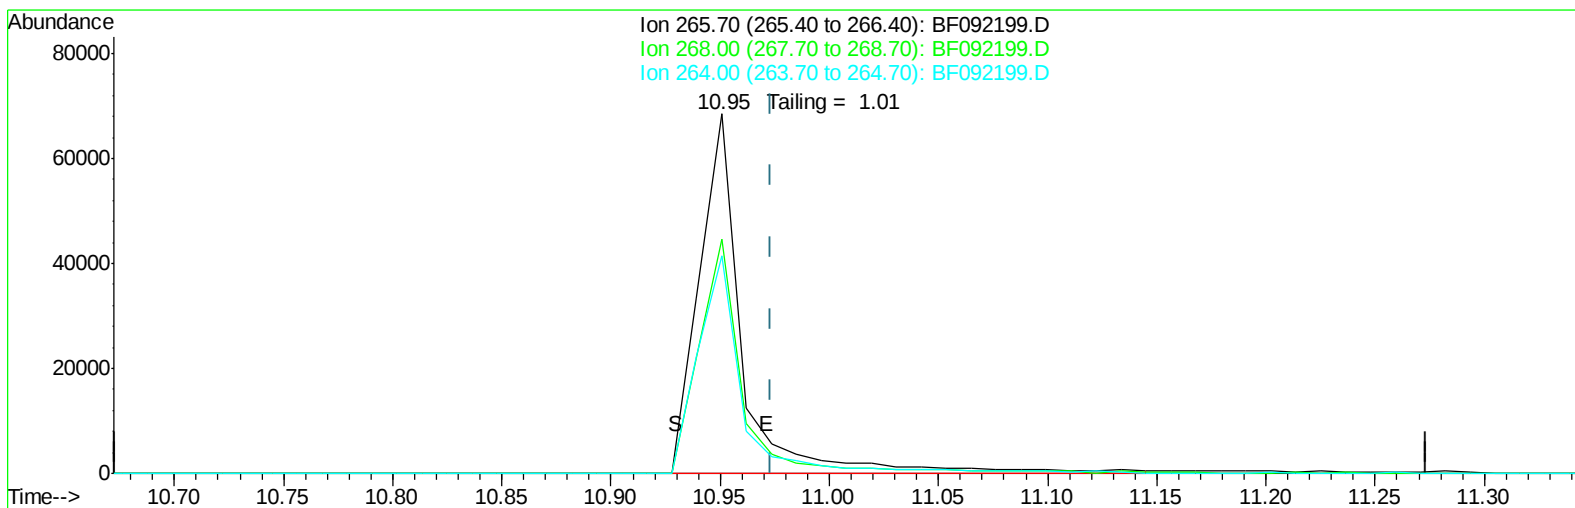

TIC: BF092199.D

(69) Pentachlorophenol (C)




10.951min (-0.023) 0.00ng

response 95488

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	65.25
264.00	62.90	60.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF011117\
Data File : BF092199.D
Acq On : 11 Jan 2017 15:07
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 14:27:49 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

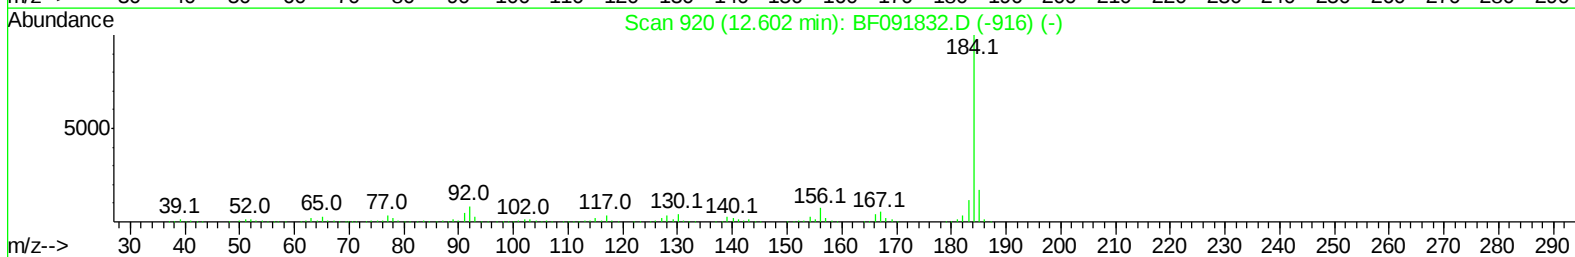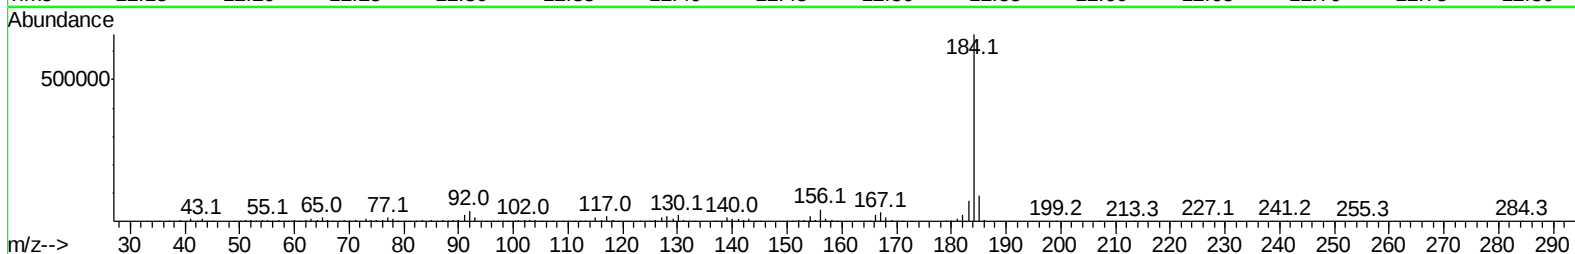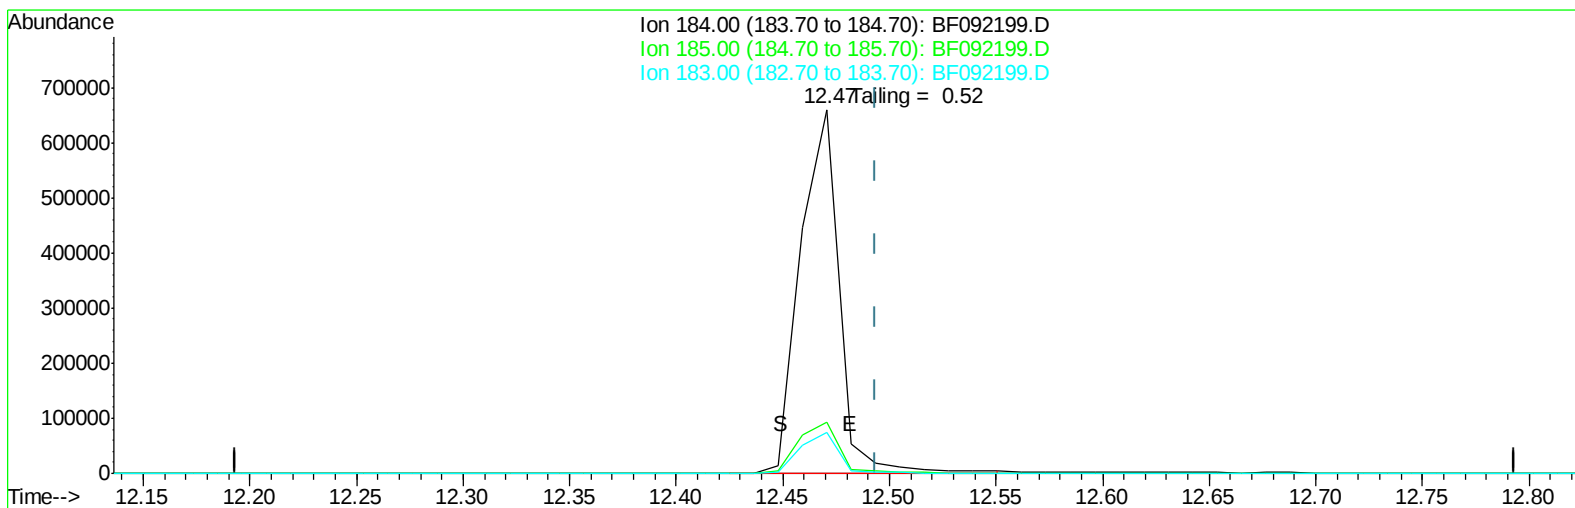

TIC: BF092199.D

(76) Benzidine

12.471min (-0.023) 0.00ng

response 858951

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.00
183.00	11.50	11.12
0.00	0.00	0.00