


Data Path : Z:\HPCHEM1\BNA F\DATA\BF011117\
 Data File : BF092199.D
 Acq On : 11 Jan 2017 15:07
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 06 15:43:51 2017

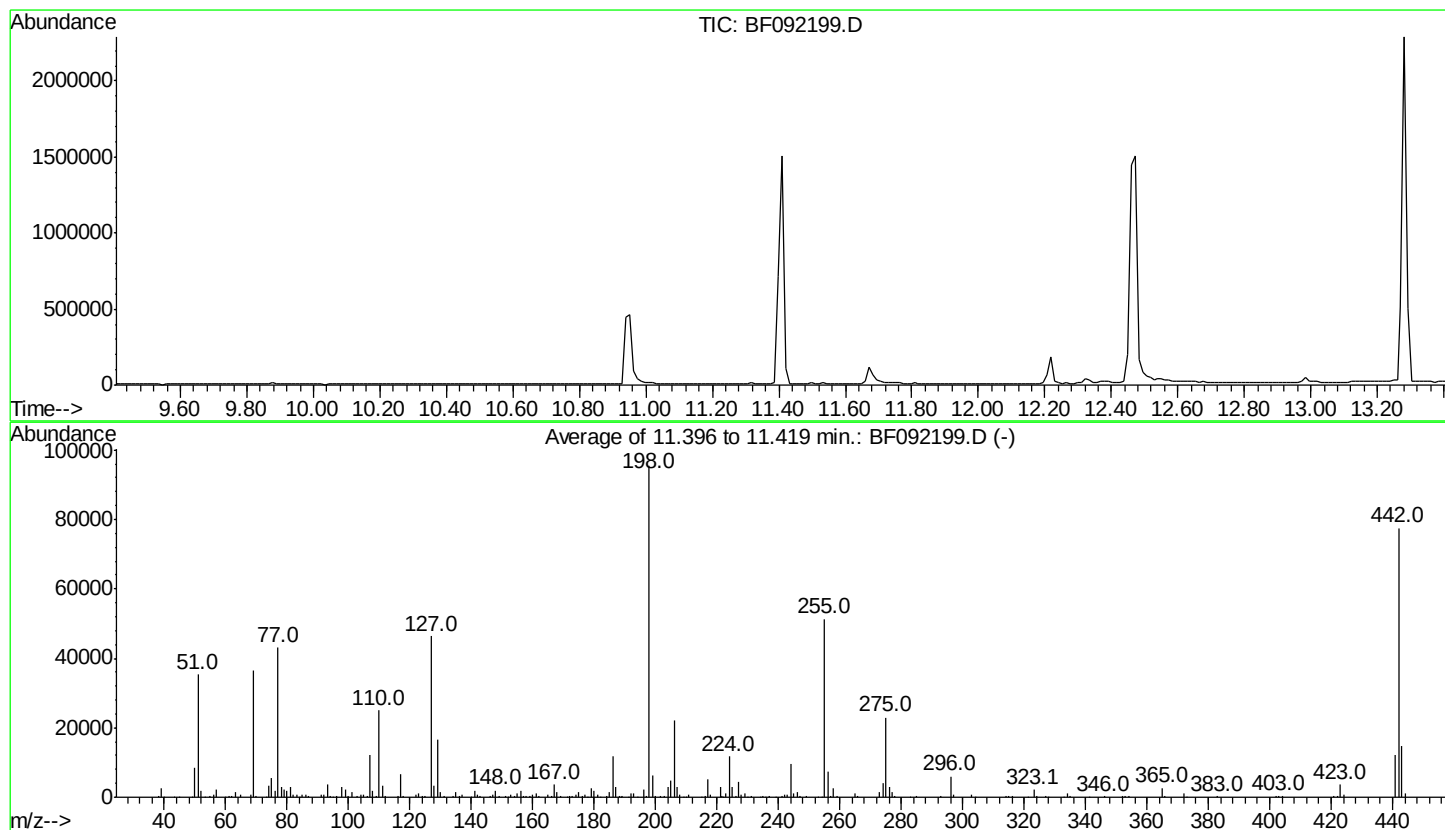

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	35350	PASS
68	69	0.00	2	1.7	626	PASS
69	198	0.00	100	38.2	36507	PASS
70	69	0.00	2	0.6	227	PASS
127	198	10	80	48.5	46295	PASS
197	198	0.00	2	0.5	513	PASS
198	198	100	100	100.0	95501	PASS
199	198	5	9	6.6	6269	PASS
275	198	10	60	24.0	22884	PASS
365	198	1	100	2.8	2650	PASS
441	442	0.01	24	15.7	12198	PASS
442	198	50	100	81.2	77509	PASS
443	442	15	24	19.1	14773	PASS