

Data Path : U:\HPCHEM1\BNA F\DATA\BF011118\
 Data File : BF102031.D
 Acq On : 11 Jan 2018 21:00
 Operator : SJ/JU
 Sample : J1062-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-28-COMP

Quant Time: Jan 11 23:44:31 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 11 12:53:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	219008	20.00	ng	0.00
21) Naphthalene-d8	8.00	136	886811	20.00	ng	0.00
38) Acenaphthene-d10	9.76	164	373902	20.00	ng	0.00
63) Phenanthrene-d10	11.24	188	584214	20.00	ng	0.00
75) Chrysene-d12	13.87	240	346955	20.00	ng	0.00
86) Perylene-d12	15.29	264	387292	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.34	112	1320925	85.17	ng	0.01
7) Phenol-d6	6.36	99	1572992	85.01	ng	0.00
23) Nitrobenzene-d5	7.29	82	998063	66.14	ng	0.00
41) 2,4,6-Tribromophenol	10.55	330	291681	89.39	ng	0.00
44) 2-Fluorobiphenyl	9.09	172	1457042	60.88	ng	0.00
78) Terphenyl-d14	12.83	244	979731	58.63	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	6.37	94	71424	3.415	ng	88
19) n-Nitroso-di-n-propylamine	7.29	70	134089	11.057	ng	# 82
25) Isophorone	7.29	82	998042	33.470	ng	# 64
49) Dimethylphthalate	9.48	163	157284	5.244	ng	98
56) 2,4-Dinitrotoluene	9.76	165	48567	6.467	ng	# 23
62) Azobenzene	10.47	77	91266	3.074	ng	# 1
64) 4,6-Dinitro-2-methylphenol	10.55	198	681	5.851	ng	# 1
66) 4-Bromophenyl-phenylether	10.55	248	18763	3.041	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA F\DATA\BF011118\
Data File : BF102031.D
Acq On : 11 Jan 2018 21:00
Operator : SJ/JU
Sample : J1062-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-28-COMP

Quant Time: Jan 11 23:44:31 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

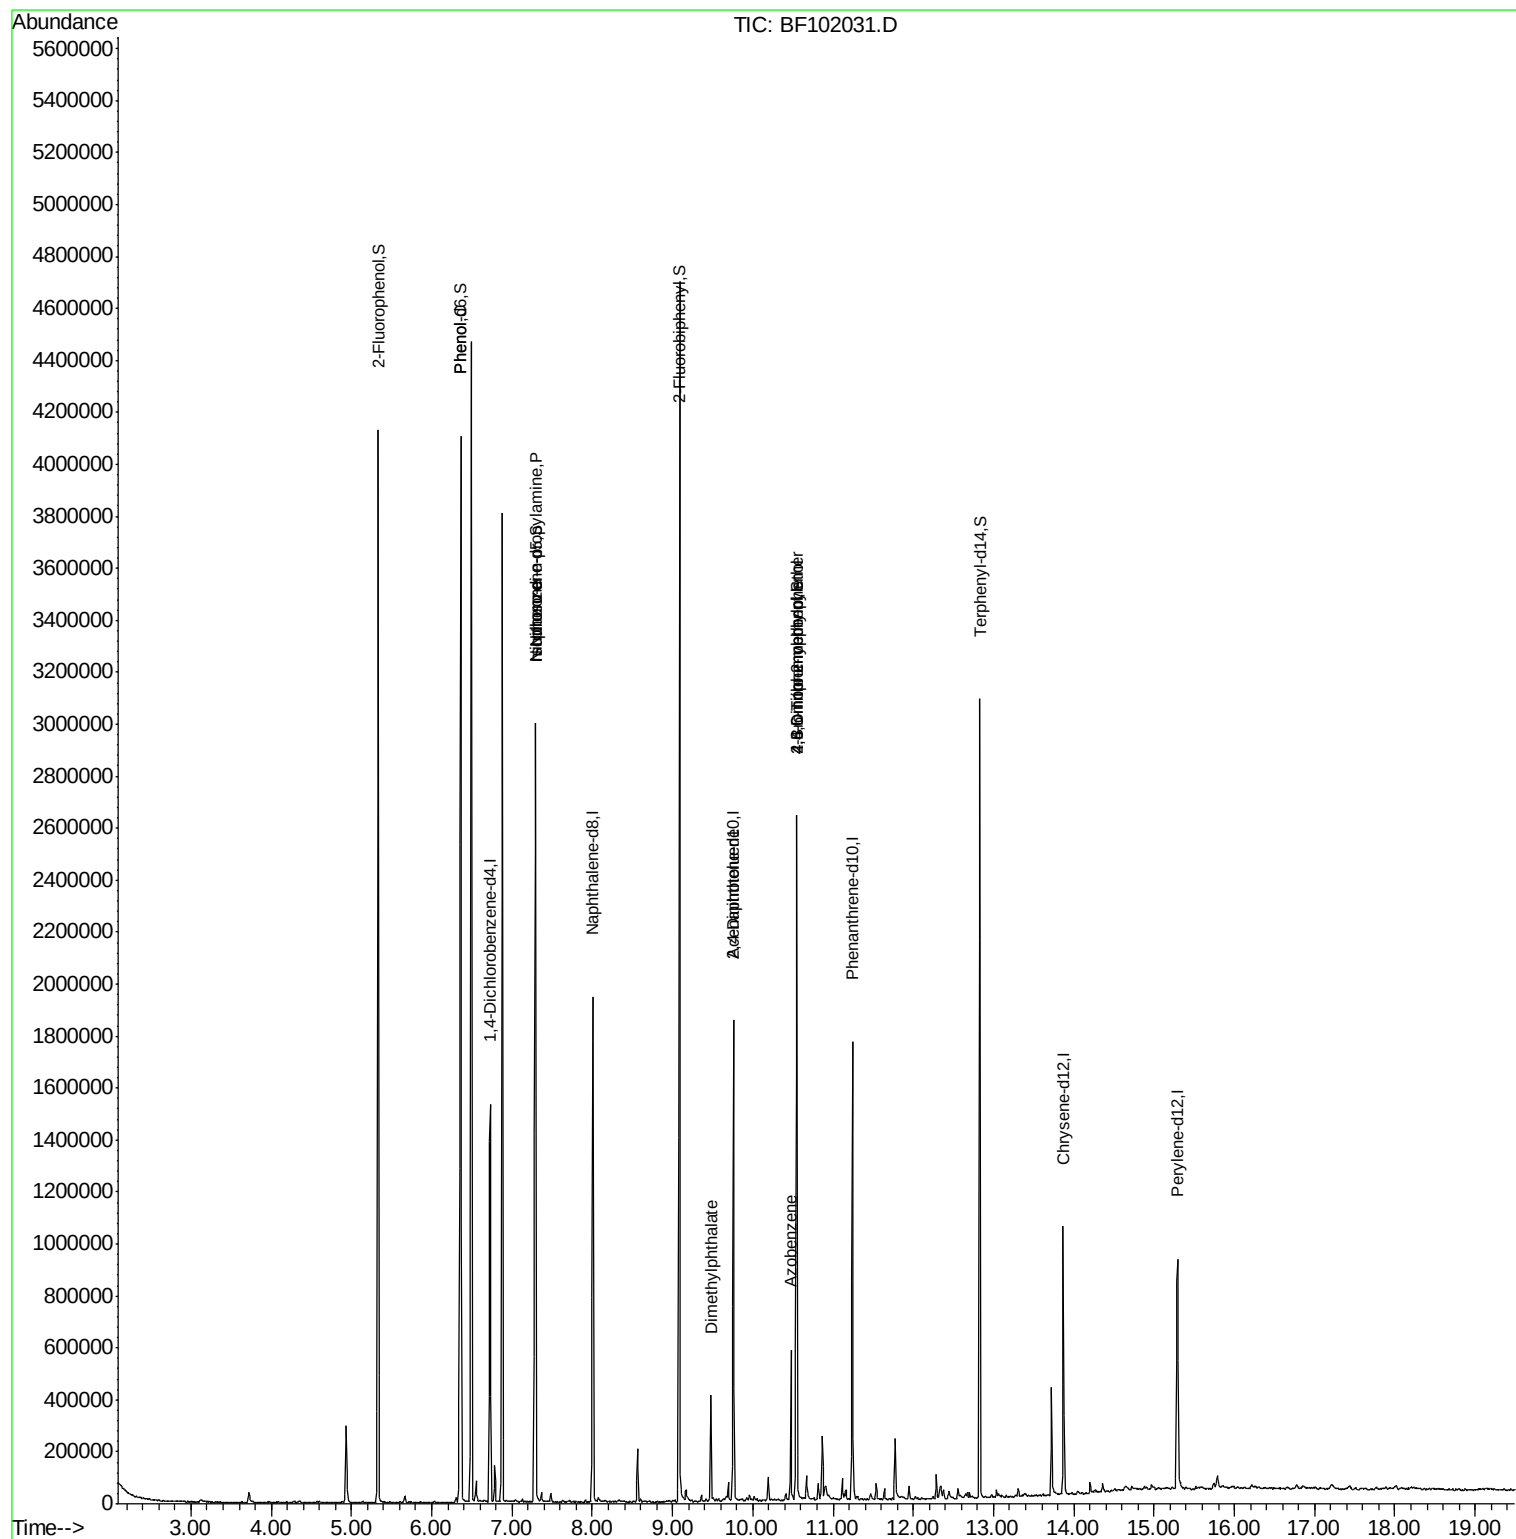




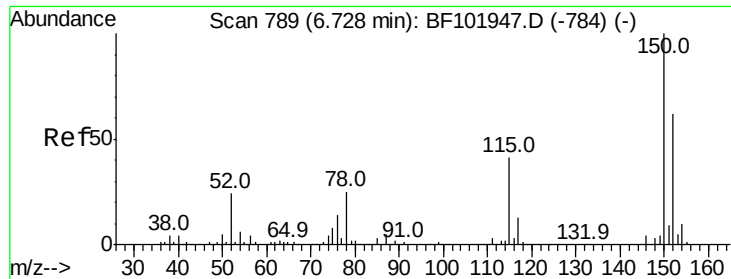


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.73 min Scan# 789
Delta R.T. 0.00 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00

Instrument :
BNA_F
ClientSampleId :
SB-28-COMP




Tot Ion:152 Resp: 219008
Ion Ratio Lower Upper
152 100
150 151.9 124.6 186.8
115 60.2 50.1 75.1

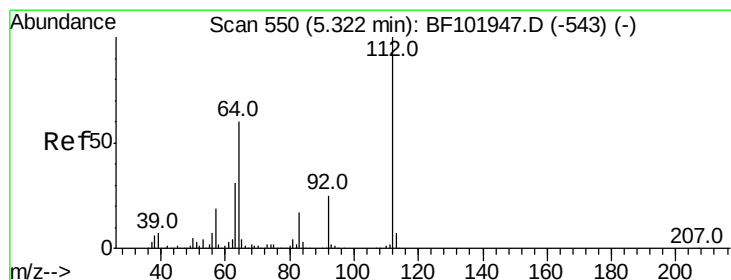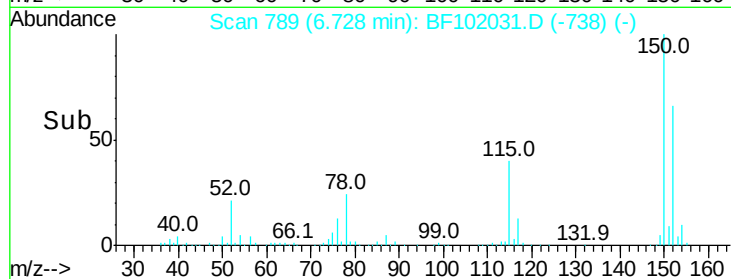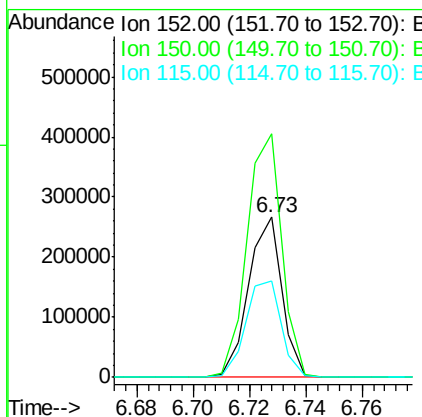


#5

2-Fluorophenol
Concen: 85.168 ng
RT: 5.34 min Scan# 553
Delta R.T. 0.01 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00

Tgt Ion:112 Resp: 1320925
Ion Ratio Lower Upper
112 100
64 58.1 47.9 71.9
63 29.5 23.7 35.5

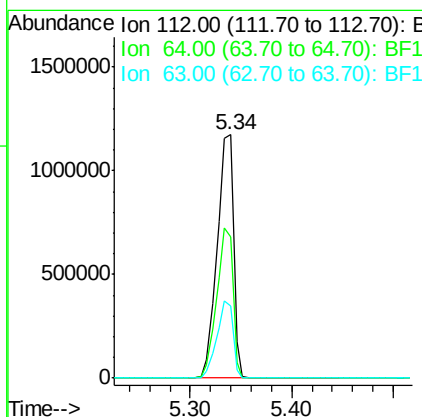

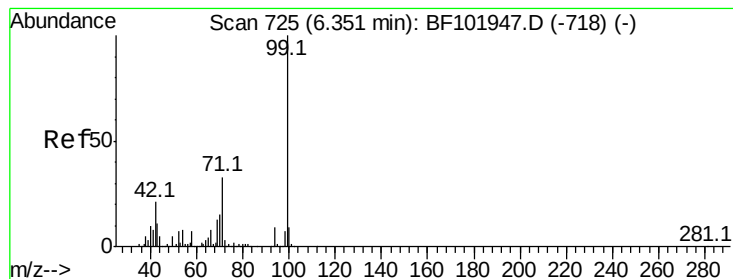

#7

Phenol-d6

Concen: 85.006 ng

RT: 6.36 min Scan# 727

Delta R.T. 0.00 min

Lab File: BF102031.D

Acq: 11 Jan 2018 21:00

Instrument :


BNA_F

ClientSampleId :

SB-28-COMP

Tot Ion: 99 Resp: 1572992




Ion	Ratio	Lower	Upper
99	100		
42	19.7	14.5	21.7
71	33.4	25.4	38.0

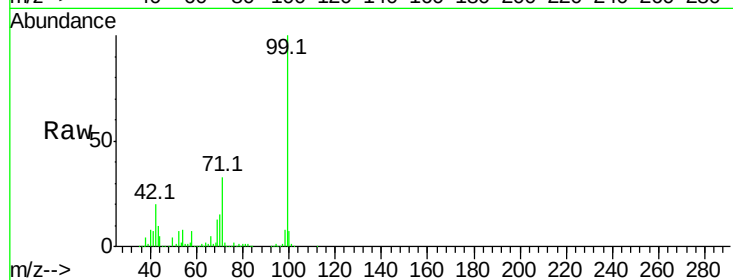

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

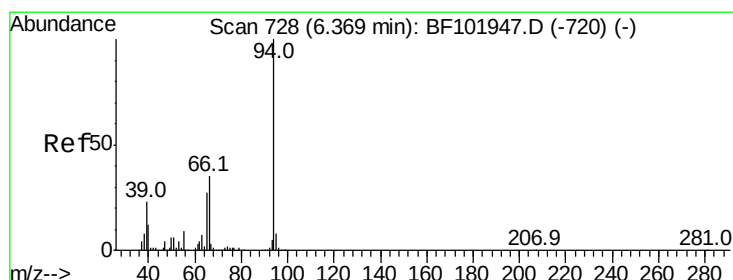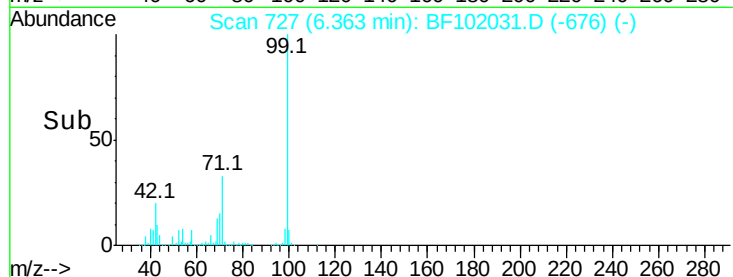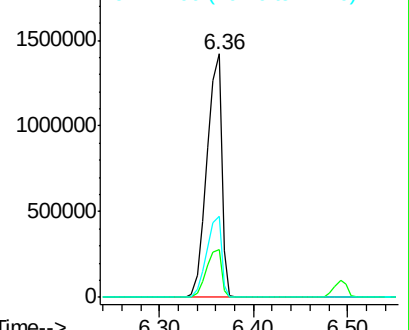

#10

Phenol

Concen: 3.415 ng

RT: 6.37 min Scan# 728


Delta R.T. -0.01 min

Lab File: BF102031.D

Acq: 11 Jan 2018 21:00

Tgt Ion: 94 Resp: 71424



Ion	Ratio	Lower	Upper
94	100		
65	31.0	7.9	47.9
66	46.2	16.2	56.2

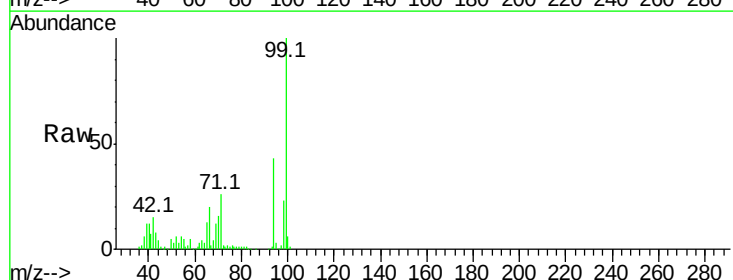


Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1



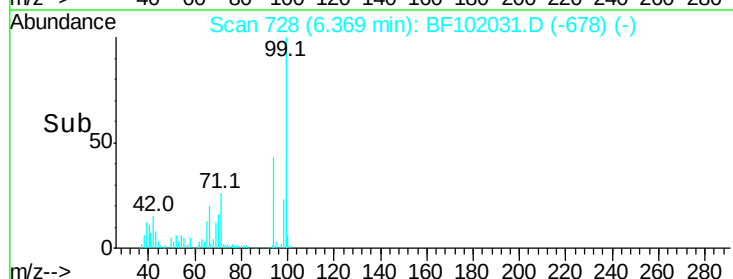
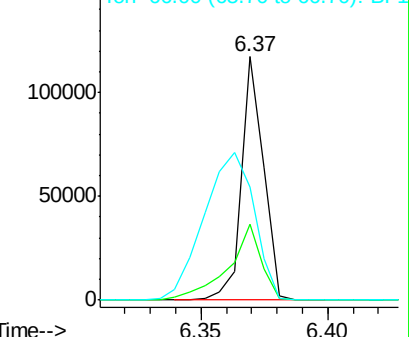




#19
n-Nitroso-di-n-propylamine
Concen: 11.057 ng
RT: 7.29 min Scan# 885
Delta R.T. 0.14 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00




Instrument :
BNA_F
ClientSampleId :
SB-28-COMP


Tot Ion: 70 Resp: 134089
Ion Ratio Lower Upper
70 100
42 52.9 47.5 71.3
101 0.0 7.4 11.2#
130 1.8 16.6 25.0#

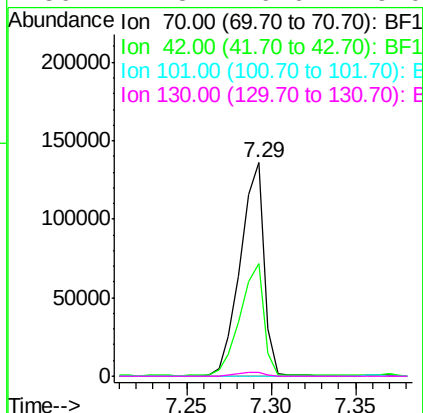

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.00 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00

Tgt Ion: 136 Resp: 886811
Ion Ratio Lower Upper
136 100
137 11.2 8.9 13.3
54 9.3 6.6 9.8
68 6.3 5.0 7.4


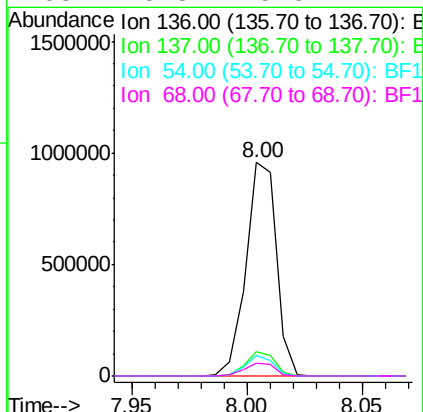






#23
 Nitrobenzene-d5
 Concen: 66.136 ng
 RT: 7.29 min Scan# 885
 Delta R.T. -0.01 min
 Lab File: BF102031.D
 Acq: 11 Jan 2018 21:00




Instrument :
 BNA_F
 ClientSampleId :
 SB-28-COMP


Tot Ion	82	Resp	998063
Ion Ratio	Lower	Upper	
82	100		
128	46.6	36.1	54.1
54	54.1	41.4	62.2

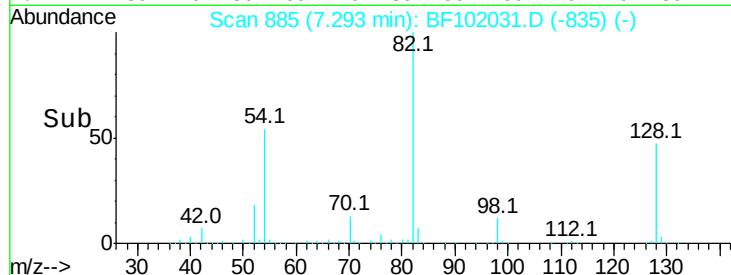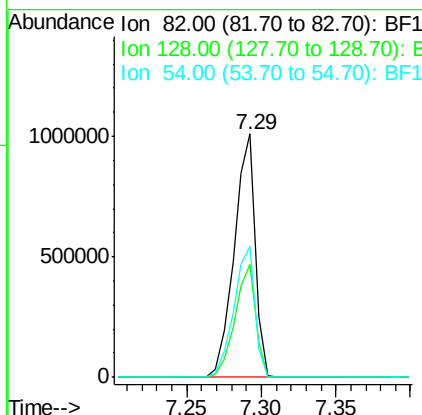

#25
 Isophorone
 Concen: 33.470 ng
 RT: 7.29 min Scan# 885
 Delta R.T. -0.26 min
 Lab File: BF102031.D
 Acq: 11 Jan 2018 21:00

Tgt Ion	82	Resp	998042
Ion Ratio	Lower	Upper	
82	100		
95	0.0	5.2	7.8#
138	0.0	14.9	22.3#

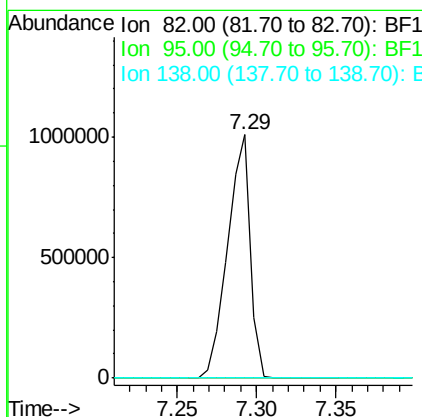



#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.76 min Scan# 1304

Delta R.T. -0.01 min

Lab File: BF102031.D

Acq: 11 Jan 2018 21:00

Instrument :

BNA_F

ClientSampleId :

SB-28-COMP


Tot Ion:164 Resp: 373902

Ion Ratio Lower Upper

164 100

162 104.1 86.1 129.1




160 45.7 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

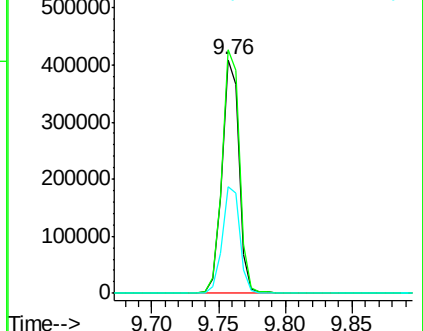

#41

2,4,6-Tribromophenol

Concen: 89.391 ng

RT: 10.55 min Scan# 1438

Delta R.T. -0.01 min

Lab File: BF102031.D

Acq: 11 Jan 2018 21:00


Tgt Ion:330 Resp: 291681

Ion Ratio Lower Upper

330 100

332 98.1 77.0 115.6



141 38.2 29.9 44.9




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

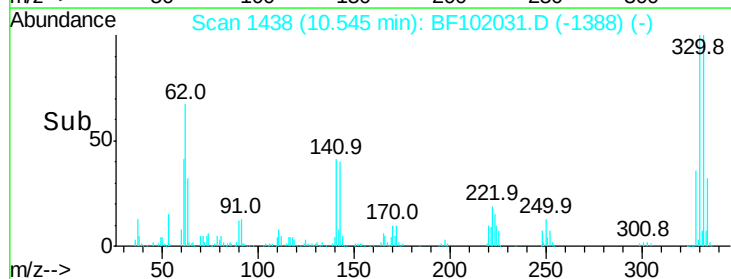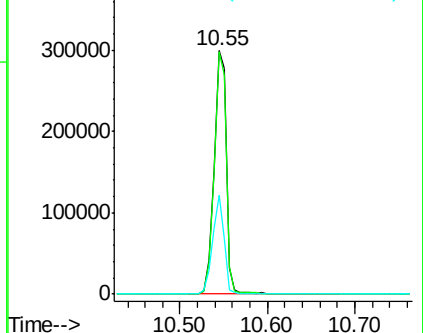


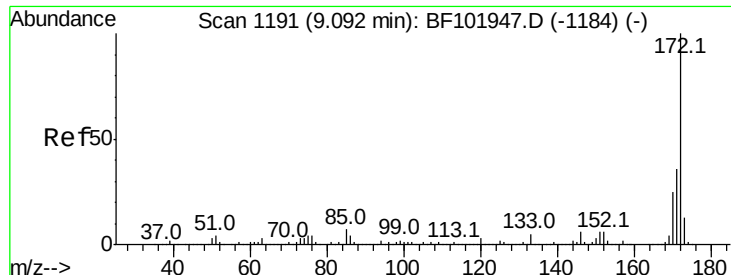




#44
2-Fluorobiphenyl
Concen: 60.879 ng
RT: 9.09 min Scan# 1190
Delta R.T. -0.01 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00

Instrument :
BNA_F
ClientSampleId :
SB-28-COMP

Tot Ion:172 Resp: 1457042
Ion Ratio Lower Upper
172 100
171 36.3 29.7 44.5
170 24.6 19.6 29.4




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

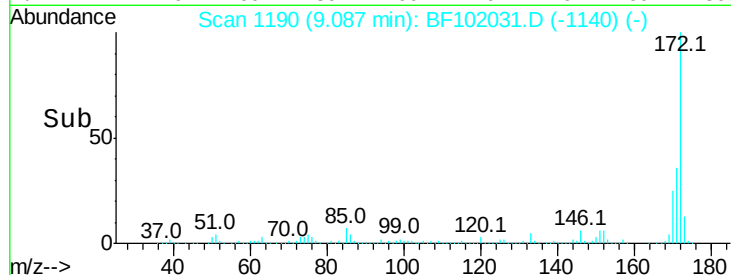
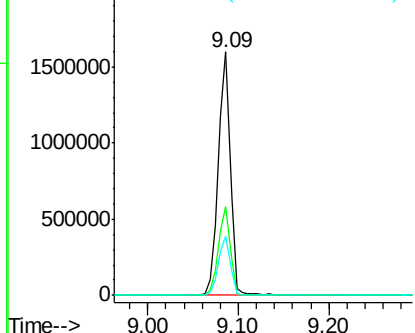



#49
Dimethylphthalate
Concen: 5.244 ng
RT: 9.48 min Scan# 1257
Delta R.T. -0.01 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00

Tgt Ion:163 Resp: 157284
Ion Ratio Lower Upper
163 100
194 3.1 2.7 4.1
164 9.4 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E



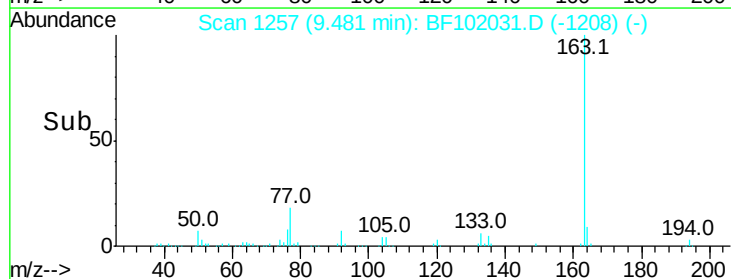
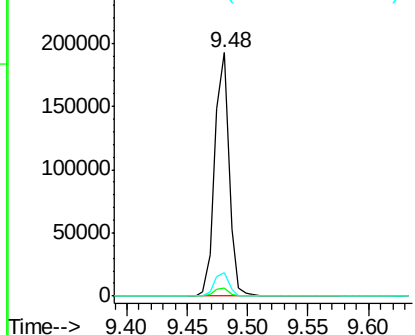




#56
2,4-Dinitrotoluene
Concen: 6.467 ng
RT: 9.76 min Scan# 1304
Delta R.T. -0.19 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00




Instrument :
BNA_F
ClientSampleId :
SB-28-COMP


Tot Ion:165 Resp: 48567
Ion Ratio Lower Upper
165 100
63 1.6 36.4 54.6#
89 1.5 57.8 86.6#
182 0.0 1.6 2.4#

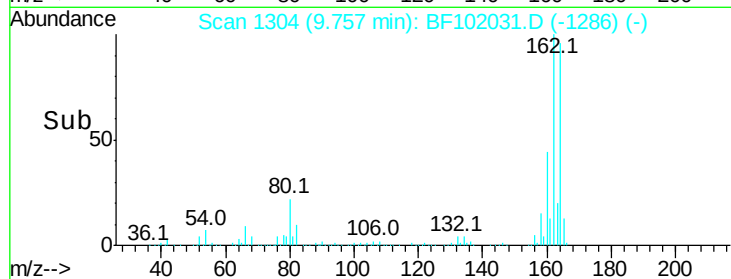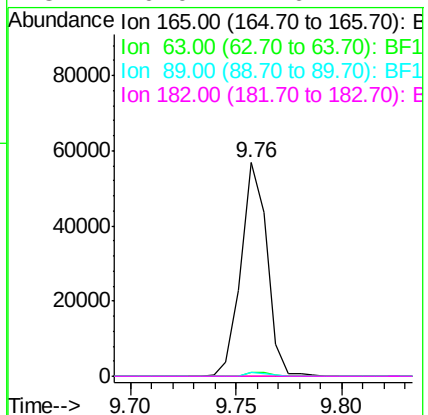

#62
Azobenzene
Concen: 3.074 ng
RT: 10.47 min Scan# 1426
Delta R.T. 0.01 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00

Tgt Ion: 77 Resp: 91266
Ion Ratio Lower Upper
77 100
182 75.4 1.7 41.7#
105 163.2 3.0 43.0#
51 40.6 9.9 49.9



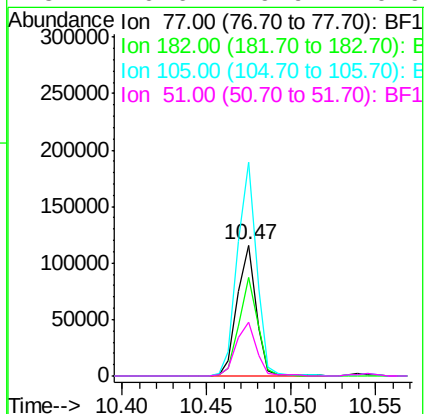





#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.24 min Scan# 1556
 Delta R.T. -0.01 min
 Lab File: BF102031.D
 Acq: 11 Jan 2018 21:00




Instrument :
 BNA_F
 ClientSampleId :
 SB-28-COMP


Tot Ion:188 Resp: 584214
 Ion Ratio Lower Upper
 188 100
 94 11.7 8.5 12.7
 80 12.7 9.2 13.8

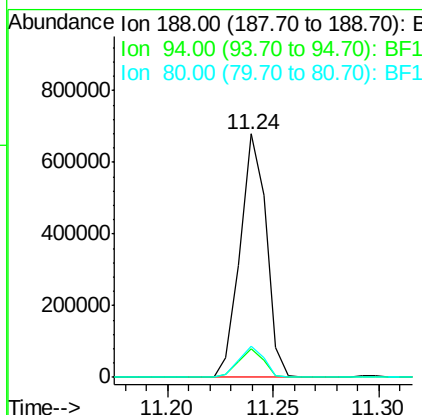

#64
 4,6-Dinitro-2-methylphenol
 Concen: 5.851 ng
 RT: 10.55 min Scan# 1438
 Delta R.T. 0.19 min
 Lab File: BF102031.D
 Acq: 11 Jan 2018 21:00

Tgt Ion:198 Resp: 681
 Ion Ratio Lower Upper
 198 100
 51 198.9 37.7 77.7#
 105 192.0 36.3 76.3#

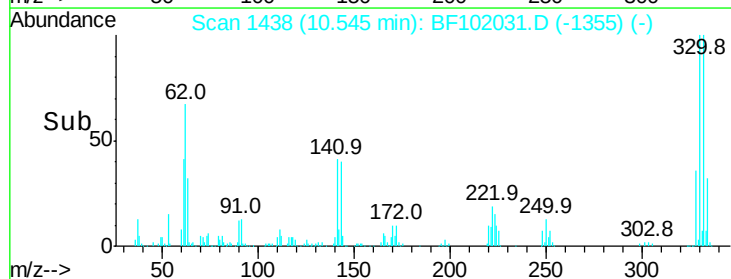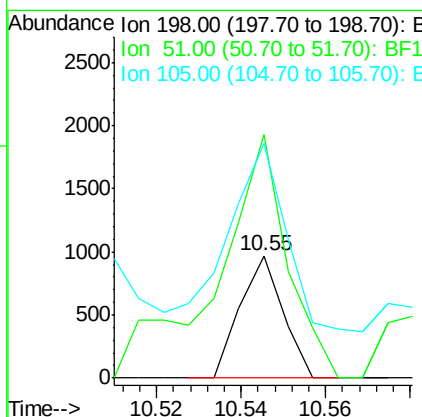


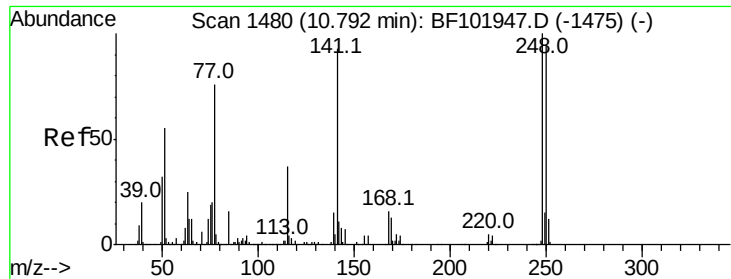




#66
4-Bromophenyl-phenylether
Concen: 3.041 ng
RT: 10.55 min Scan# 1438
Delta R.T. -0.25 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00

Instrument :
BNA_F
ClientSampleId :
SB-28-COMP

Tot Ion:248 Resp: 18763
Ion Ratio Lower Upper
248 100
250 186.5 76.9 115.3#
141 577.4 74.4 111.6#




Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E


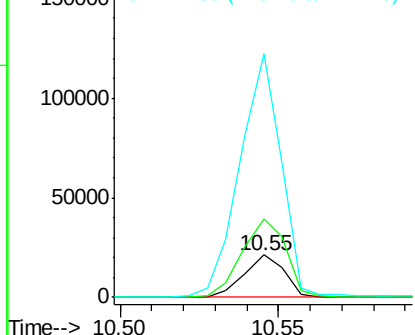



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.87 min Scan# 2004
Delta R.T. -0.01 min
Lab File: BF102031.D
Acq: 11 Jan 2018 21:00

Tgt Ion:240 Resp: 346955
Ion Ratio Lower Upper
240 100
120 12.4 9.5 14.3
236 25.9 20.7 31.1



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

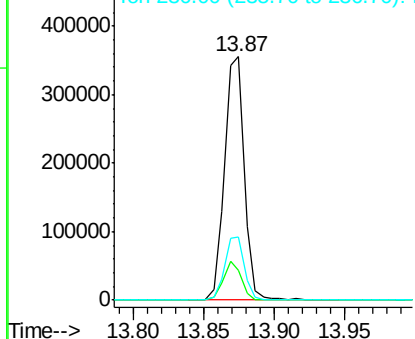

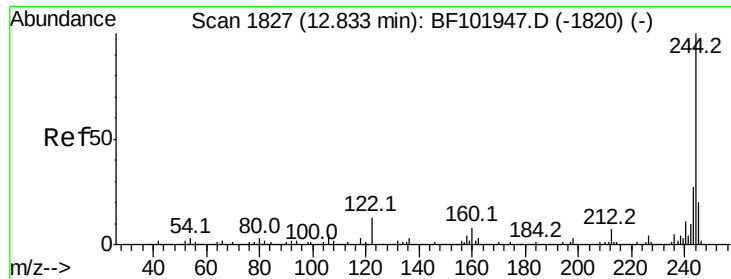

#78

Terphenyl-d14

Concen: 58.629 ng

RT: 12.83 min Scan# 1826

Delta R.T. -0.01 min

Lab File: BF102031.D

Acq: 11 Jan 2018 21:00

Instrument :

BNA_F

ClientSampleId :

SB-28-COMP


Tot Ion:244 Resp: 979731

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0




122 14.1 11.0 16.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

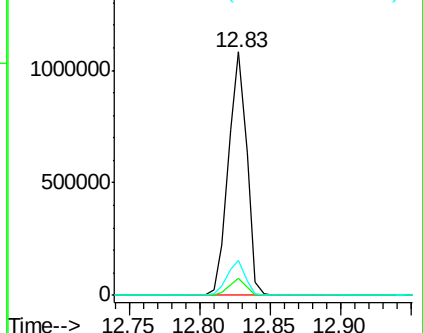

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.29 min Scan# 2245

Delta R.T. 0.00 min

Lab File: BF102031.D

Acq: 11 Jan 2018 21:00


Tgt Ion:264 Resp: 387292

Ion Ratio Lower Upper

264 100

260 22.9 19.2 28.8

265 20.3 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

