
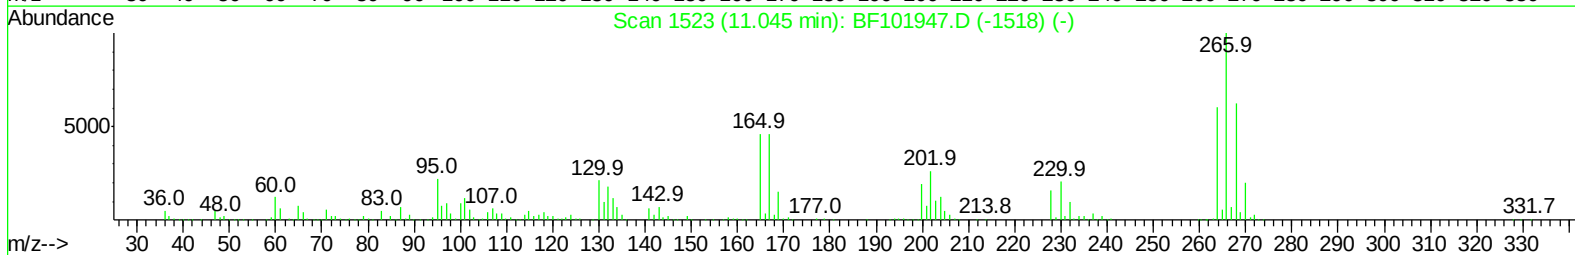
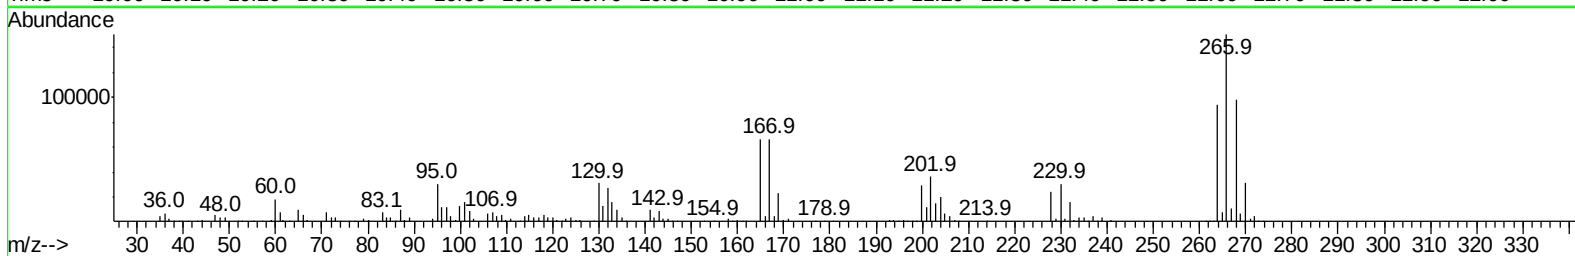


Data Path : U:\HPCHEM1\BNA F\DATA\BF011118\
Data File : BF102006.D
Acq On : 11 Jan 2018 8:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 17:11:45 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

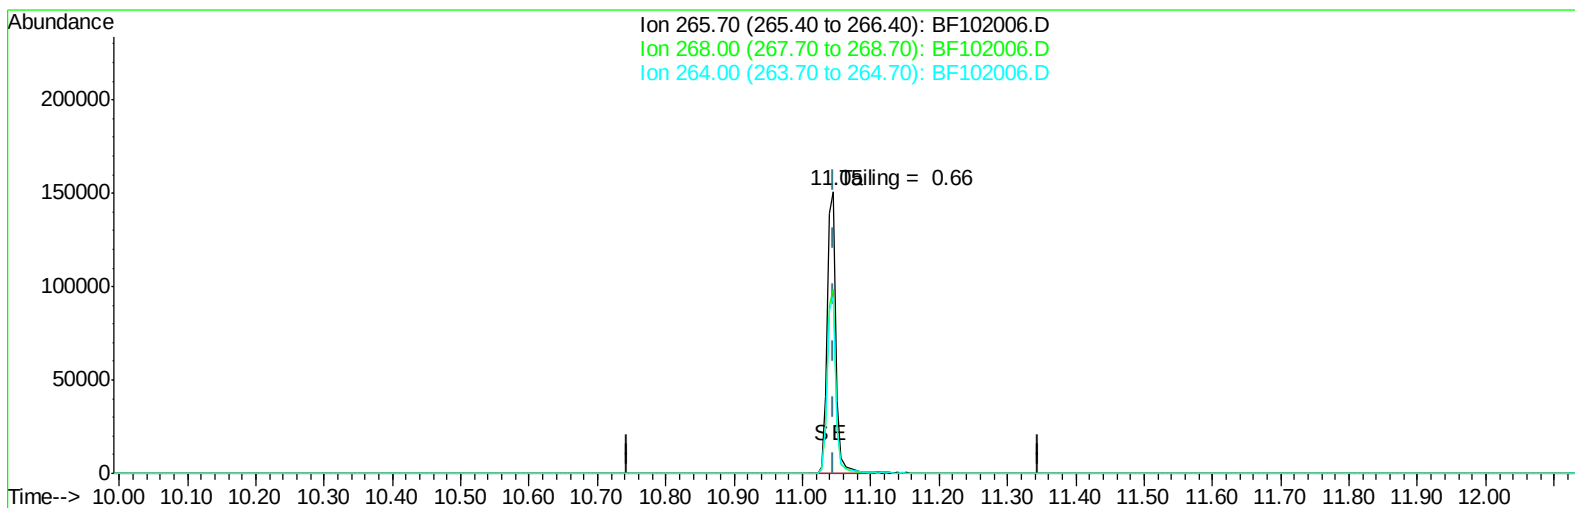

TIC: BF102006.D

(69) Pentachlorophenol (C)




11.045min (+0.000) 35921.95ng

response 140157

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.50
264.00	61.90	62.56
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA F\DATA\BF011118\
Data File : BF102006.D
Acq On : 11 Jan 2018 8:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 11 17:11:45 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 11 12:53:54 2018
Response via : Initial Calibration

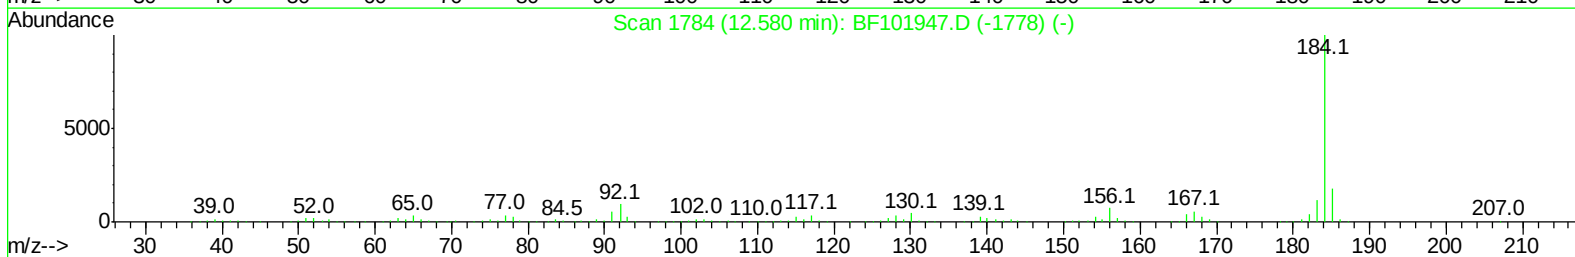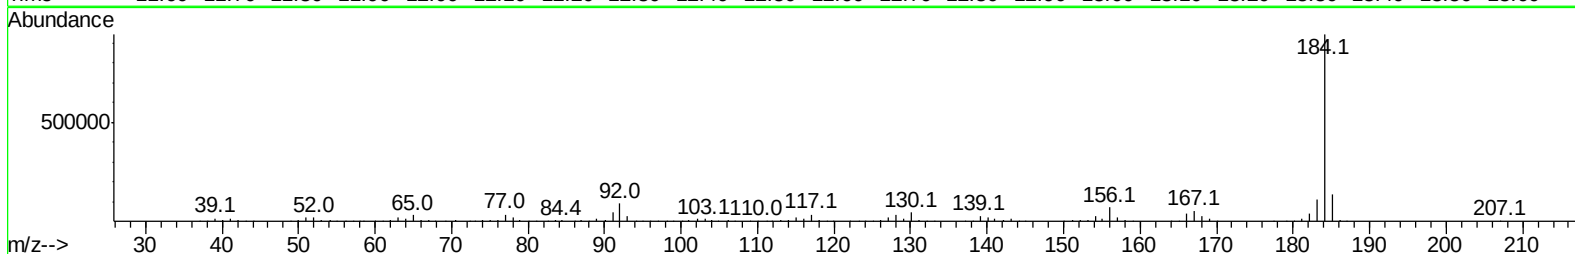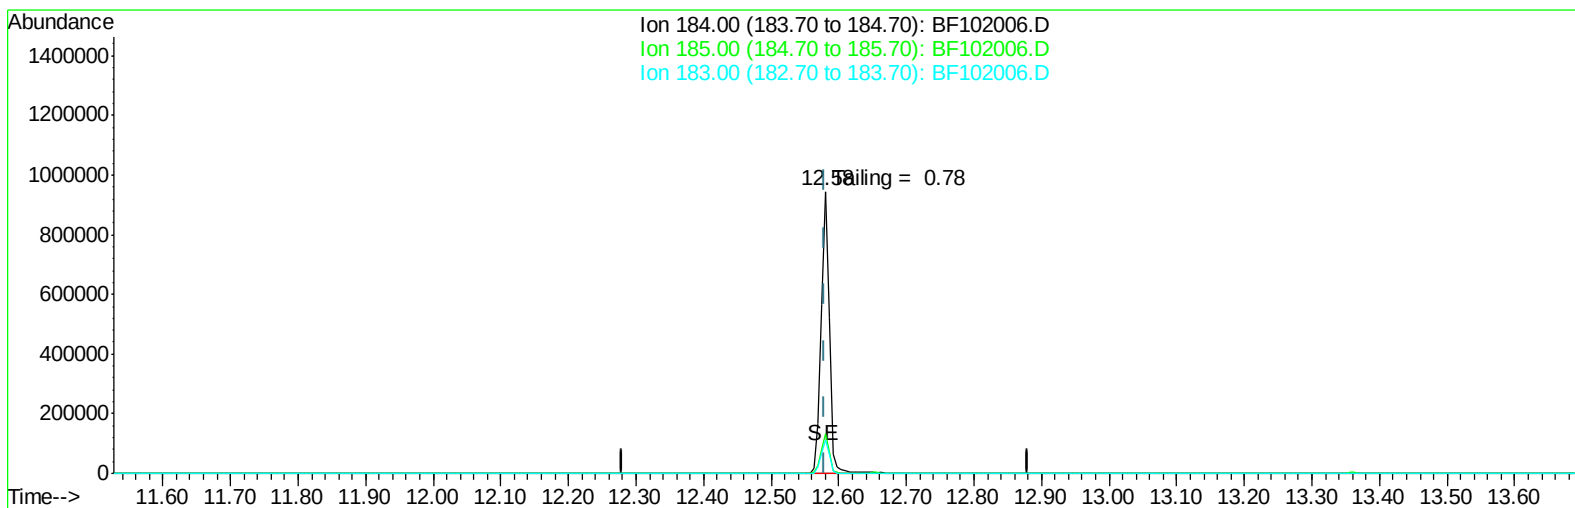

TIC: BF102006.D

(76) Benzidine

12.580min (+0.000) 0.00ng

response 833721

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.32
183.00	11.60	11.99
0.00	0.00	0.00