
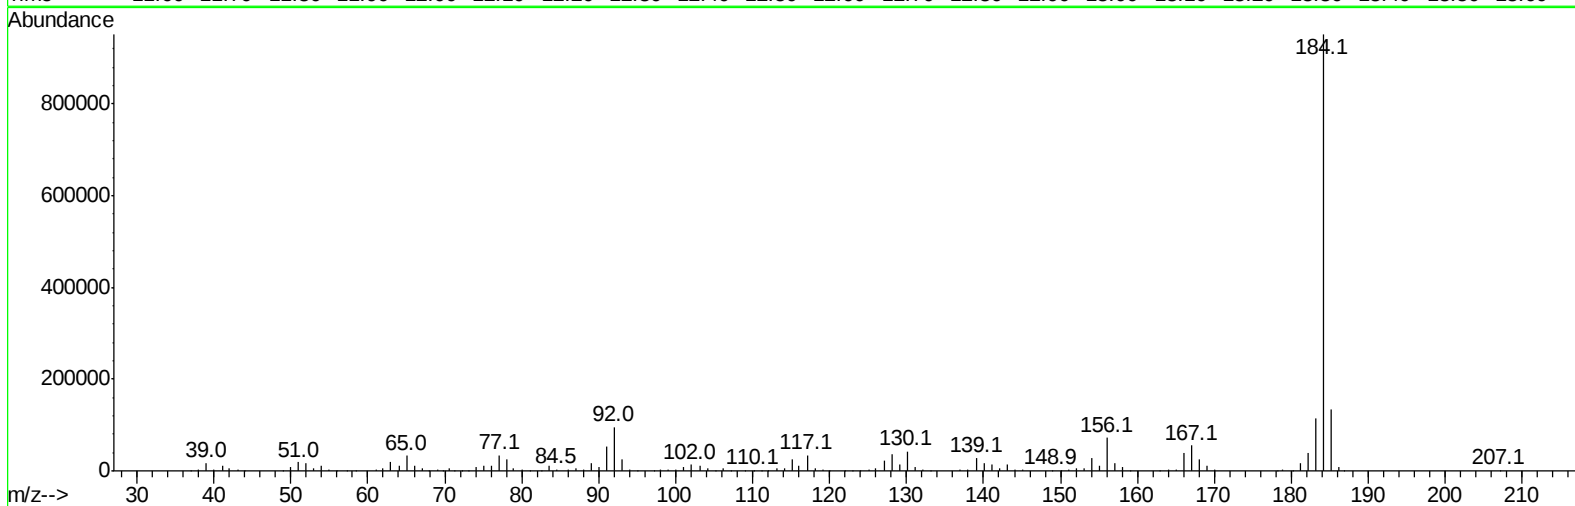


Data Path : U:\HPCHEM1\BNA F\DATA\BF011118\  
Data File : BF102017.D  
Acq On : 11 Jan 2018 14:38  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 03:35:31 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jan 11 12:53:54 2018  
Response via : Initial Calibration

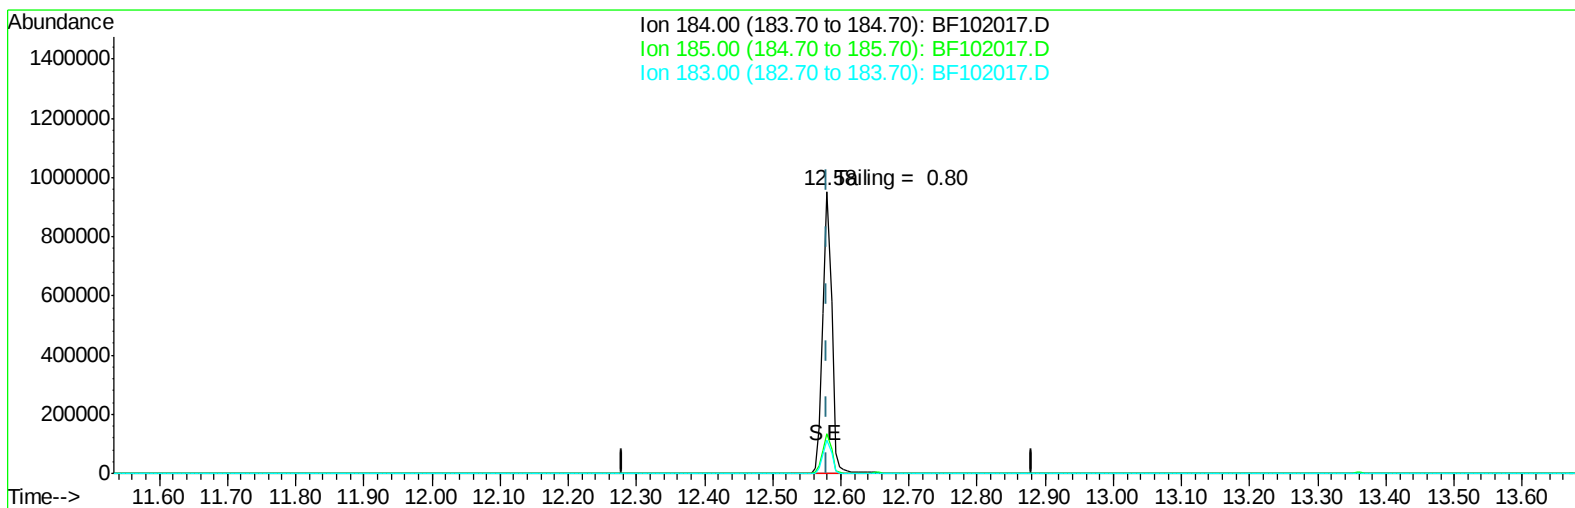

TIC: BF102017.D

(76) Benzidine



12.580min (-0.000) 0.00ng

response 844149

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.04 |
| 183.00 | 11.60 | 12.06 |
| 0.00   | 0.00  | 0.00  |

Data Path : U:\HPCHEM1\BNA F\DATA\BF011118\  
Data File : BF102017.D  
Acq On : 11 Jan 2018 14:38  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 12 03:35:31 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF010918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jan 11 12:53:54 2018  
Response via : Initial Calibration

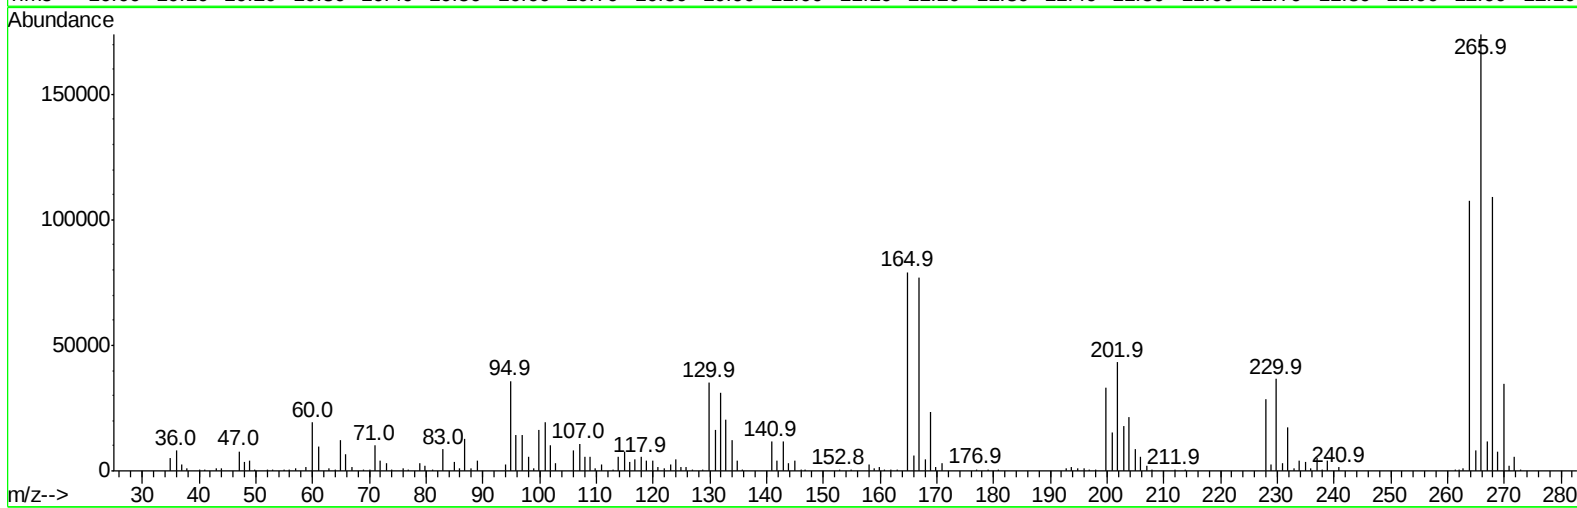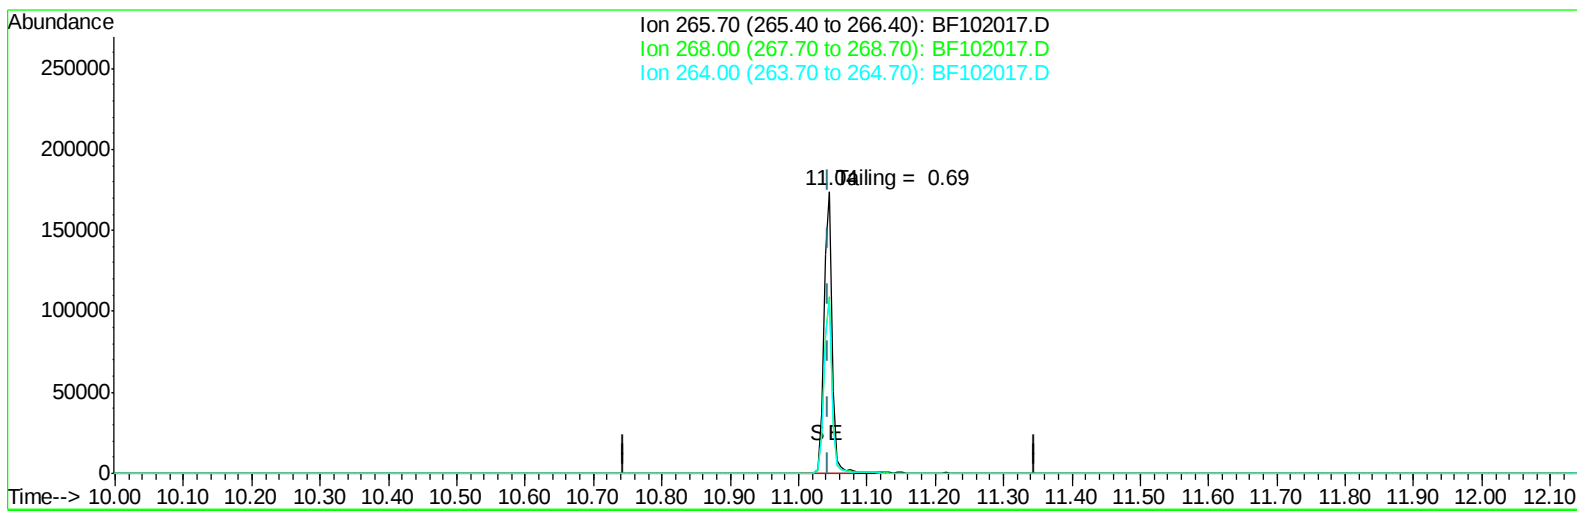

TIC: BF102017.D

(69) Pentachlorophenol (C)

11.045min (-0.000) 37220.62ng

response 149149

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 62.67 |
| 264.00 | 61.90 | 61.82 |
| 0.00   | 0.00  | 0.00  |